

Sample Name :Bradykinin (1-7)
 Cat. No. : RP11133
 Lot. No. : E4790119I
 Time Processed :8:52:26
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

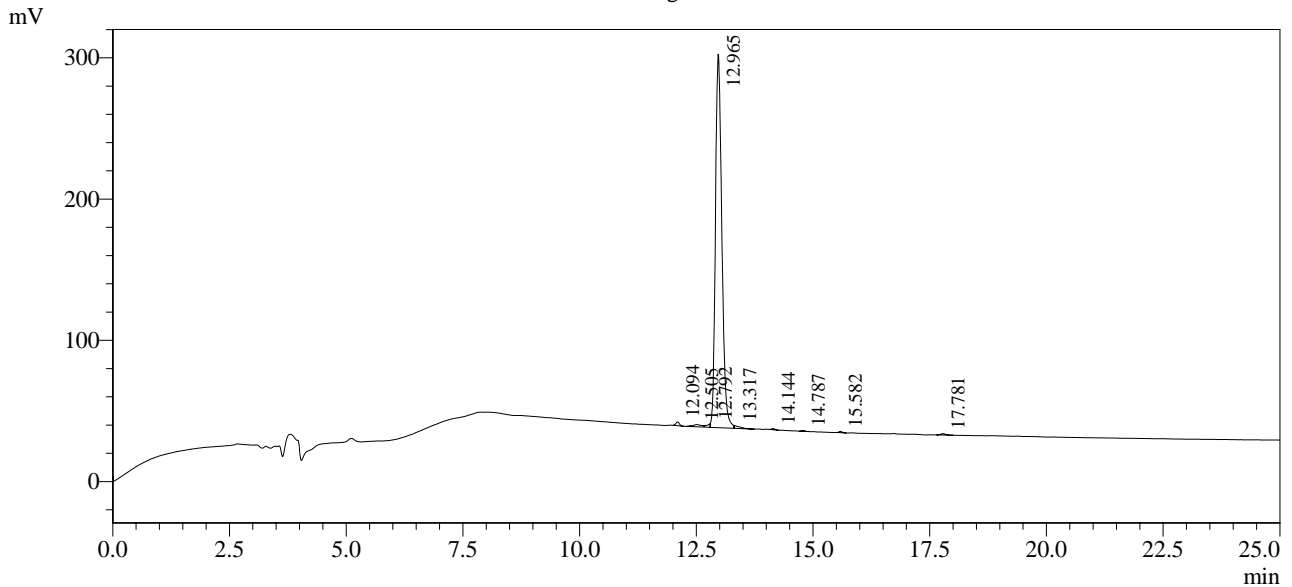

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.094	13675	2678	0.525
2	12.505	21552	1576	0.828
3	12.792	12664	2331	0.487
4	12.965	2520658	264366	96.856
5	13.317	15527	1982	0.597
6	14.144	4048	845	0.156
7	14.787	2802	572	0.108
8	15.582	4586	933	0.176
9	17.781	6958	917	0.267
Total		2602470	276200	100.000