

Sample Name : MARCKS Peptide(151-175), Phosphorylated
 Cat. No. :RP20454
 Lot. No. :E4962919I
 Time Processed :6:40:19
 Month-Day-Year Processed :09/27/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

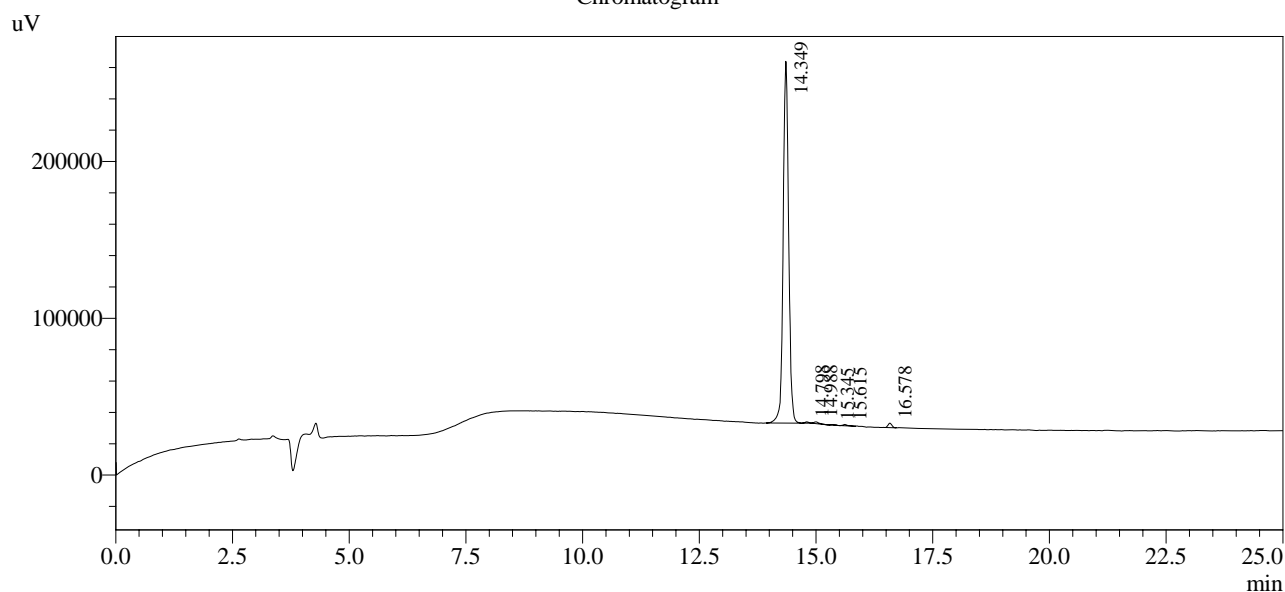

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.349	1883566	230823	98.009
2	14.798	4815	845	0.251
3	14.988	8838	1083	0.460
4	15.345	3279	354	0.171
5	15.615	5241	799	0.273
6	16.578	16082	2866	0.837
Total		1921822	236770	100.000