

Sample Name :Neuromedin B  
 Cat No :RP10507  
 Lot No :E0667721A  
 Time Processed :18:07:28  
 Month-Day-Year Processed :01/27/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK11010011

<Chromatogram>

mV

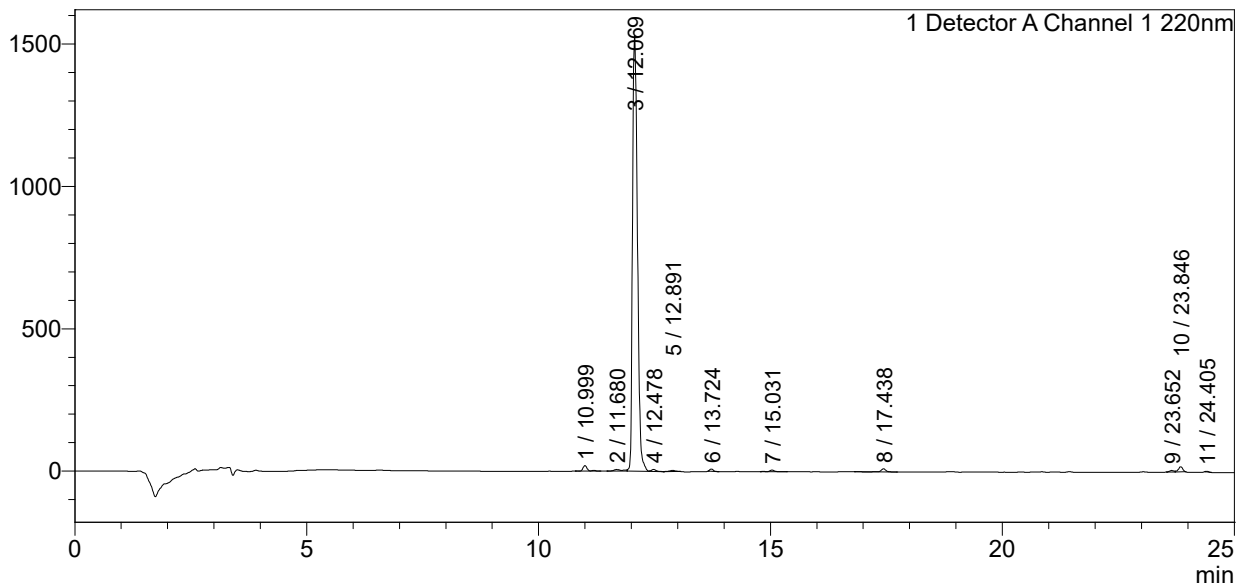

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.999	129545	19668	1.090
2	11.680	71020	5143	0.598
3	12.069	11289463	1530068	95.033
4	12.478	48678	7011	0.410
5	12.891	33076	3793	0.278
6	13.724	38477	7545	0.324
7	15.031	35652	5715	0.300
8	17.438	80863	11296	0.681
9	23.652	33214	5186	0.280
10	23.846	111318	17681	0.937
11	24.405	8220	2130	0.069
Total		11879525	1615236	100.000