

Sample Name :OVA Peptide(257-264)  
 Cat No.: RP10611  
 Lot No. :PE8861901  
 Time Processed : 9:39:00  
 Month-Day-Year Processed : 01/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

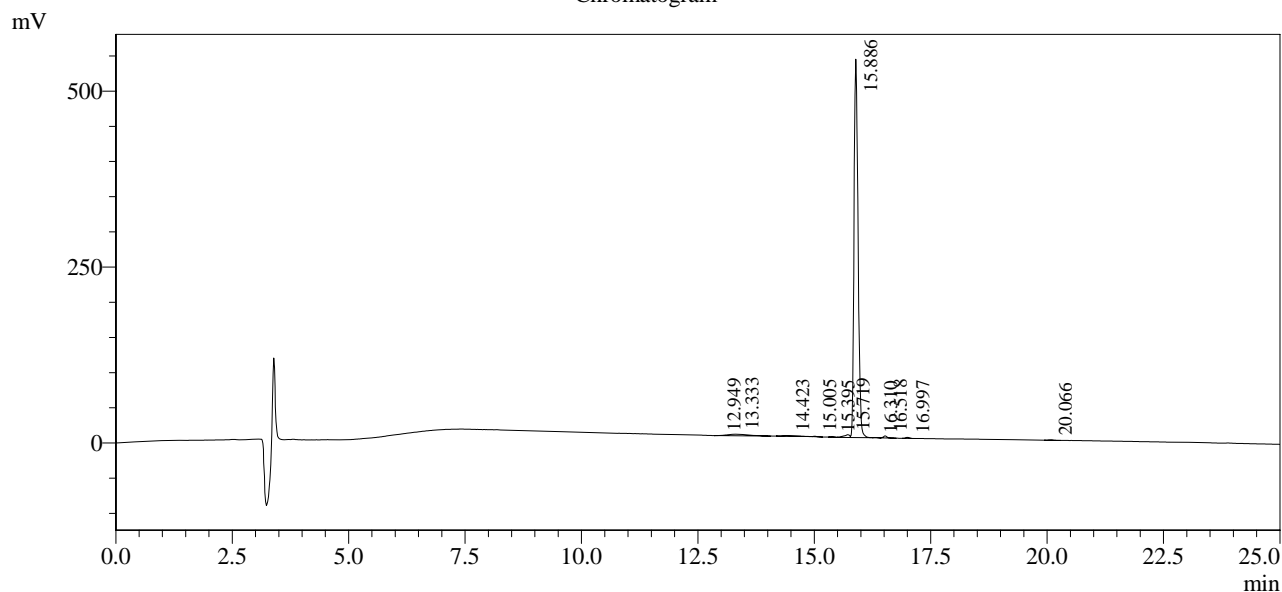

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.949	1234	253	0.036
2	13.333	72541	2350	2.135
3	14.423	16521	840	0.486
4	15.005	2810	589	0.083
5	15.395	3574	655	0.105
6	15.719	33405	3943	0.983
7	15.886	3236235	537535	95.242
8	16.310	1988	426	0.059
9	16.518	16568	2862	0.488
10	16.997	8457	1478	0.249
11	20.066	4583	643	0.135
Total		3397916	551575	100.000