

Sample Name : Cardiotoxin Analog (CTX) IV (6-12)
 Cat. No. : RP17303 Lot. No. : PE3161805


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

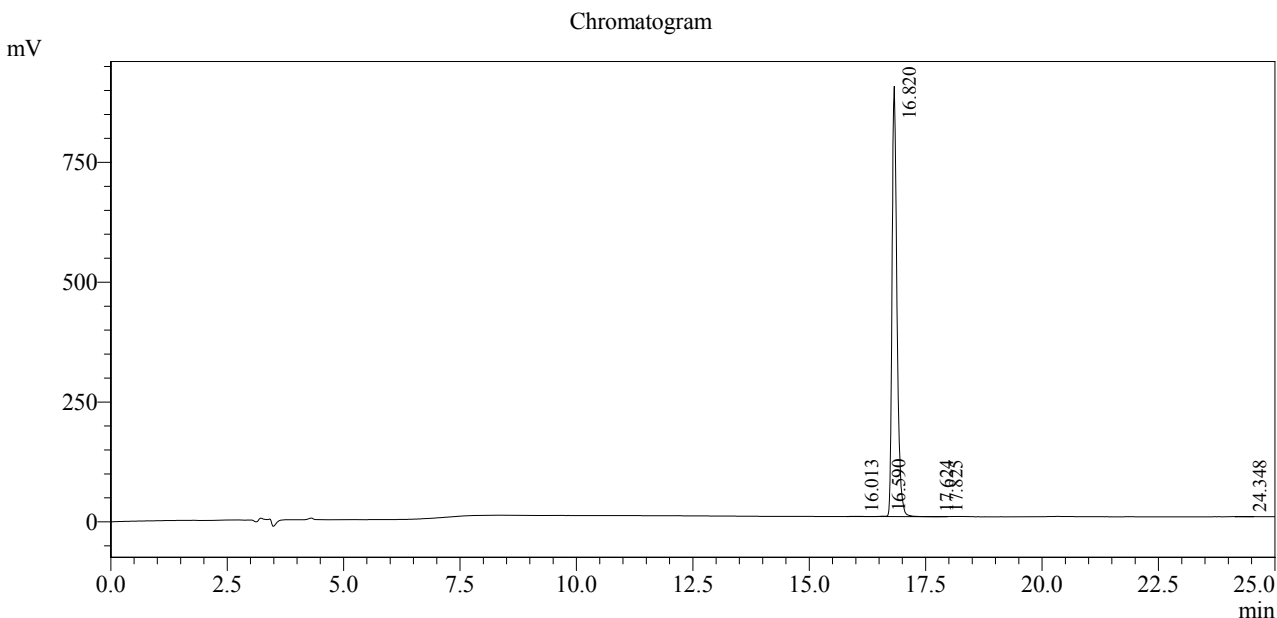

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.013	6231	416	0.094
2	16.590	6615	714	0.100
3	16.820	6625586	897535	99.675
4	17.624	2839	283	0.043
5	17.825	1362	237	0.020
6	24.348	4526	447	0.068
Total		6647159	899633	100.000