

Sample Name :BNP (1-32), rat
Cat No. : RP11121
Lot No. : PE5331902
Time Processed : 23:48:10
Month-Day-Year Processed : 02/27/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment:GK12010012

<Chromatogram>

mV

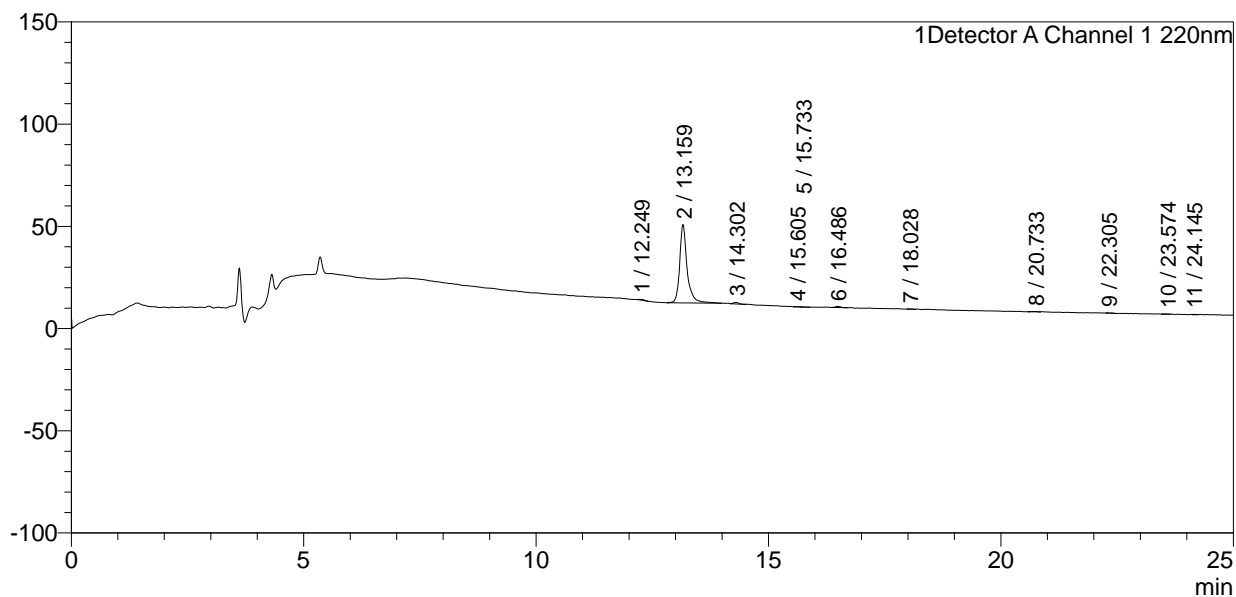

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.249	2574	353	0.577
2	13.159	426025	38358	95.487
3	14.302	5556	810	1.245
4	15.605	1140	156	0.256
5	15.733	1020	156	0.229
6	16.486	4255	524	0.954
7	18.028	1001	191	0.224
8	20.733	1351	164	0.303
9	22.305	1128	109	0.253
10	23.574	1035	150	0.232
11	24.145	1074	189	0.241
Total		446160	41159	100.000