

Sample Name :Neurotensin (8-13)
Sample ID :U683MEC100-1
Time Processed: 1:05:56
Month-Day-Year Processed :03/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Equipment:ZJ17010509

<Chromatogram>

mV

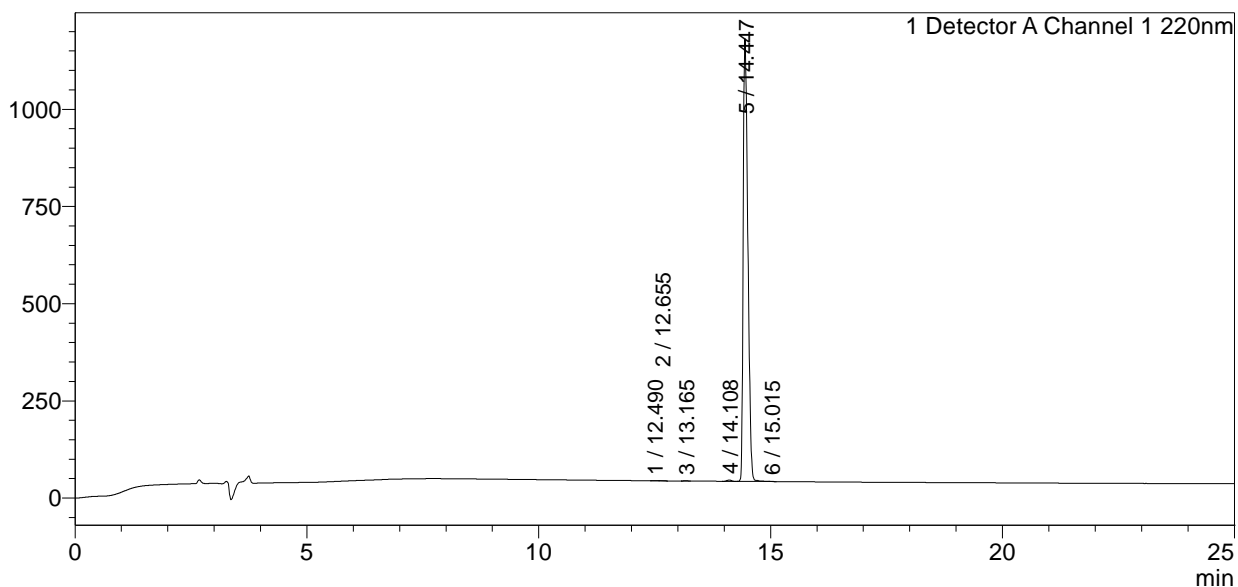

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.490	2364	545	0.030
2	12.655	2735	610	0.034
3	13.165	2521	555	0.032
4	14.108	22247	3449	0.279
5	14.447	7947121	1139107	99.607
6	15.015	1448	347	0.018
Total		7978437	1144614	100.000