

Sample Name : YRGDS Fibronectin Fragment
 Cat. No. : RP20476
 Lot. No. : PE6721710

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

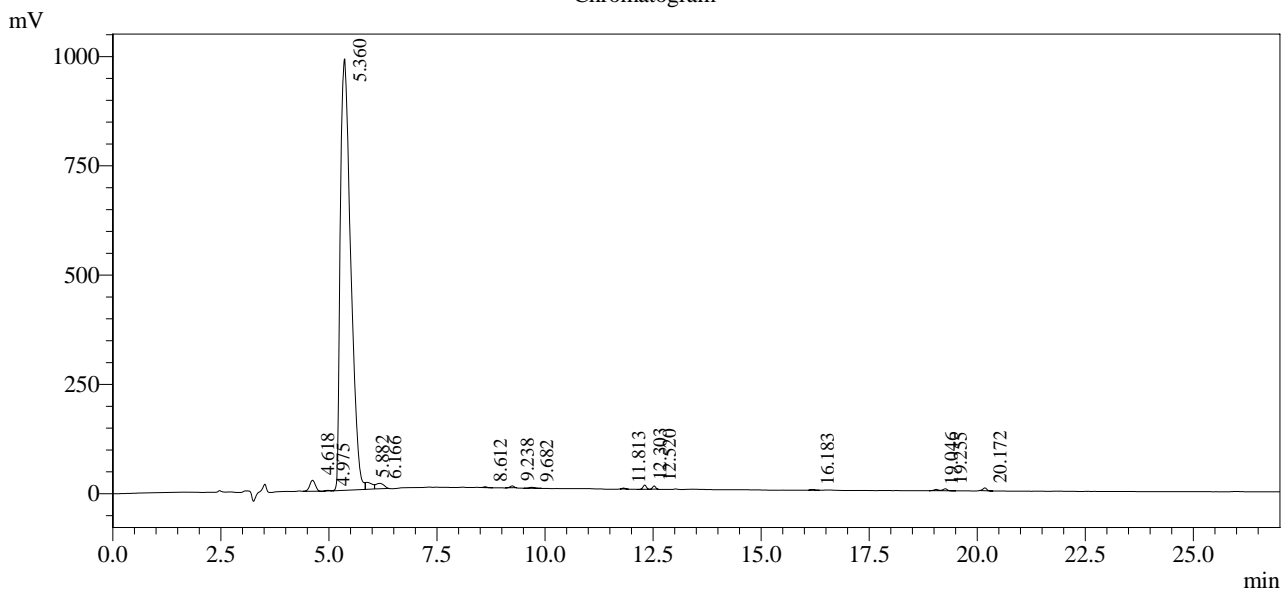

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	4.618	225732	25221	1.305
2	4.975	8812	1500	0.051
3	5.360	16477054	986953	95.232
4	5.882	172799	15953	0.999
5	6.166	161932	12566	0.936
6	8.612	10785	1996	0.062
7	9.238	26555	4208	0.153
8	9.682	19706	2356	0.114
9	11.813	10838	2167	0.063
10	12.303	49181	9630	0.284
11	12.520	33887	7200	0.196
12	16.183	8783	1555	0.051
13	19.046	21223	3073	0.123
14	19.255	34067	4561	0.197
15	20.172	40623	6509	0.235
Total		17301978	1085448	100.000