


# Mass Spectrum

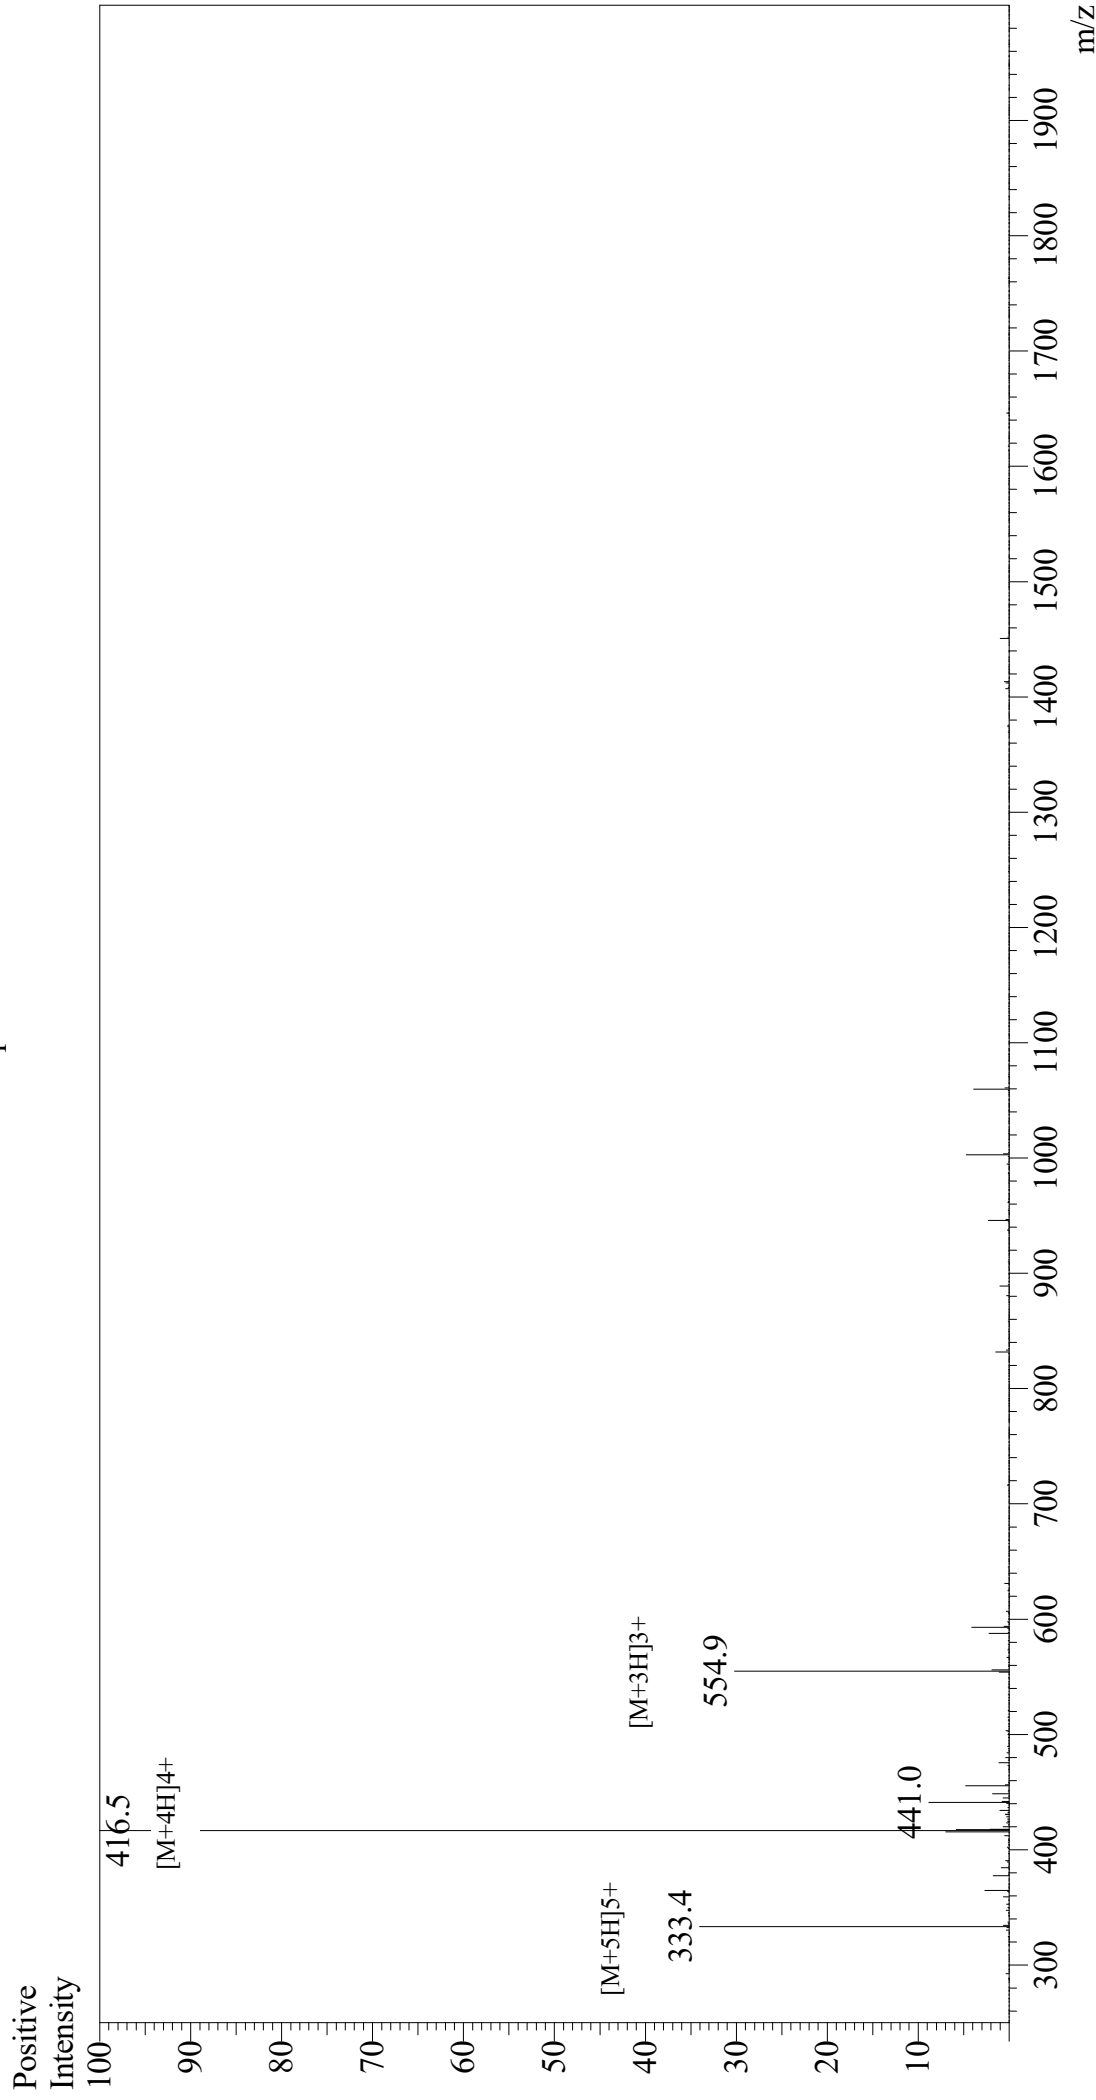

Sample Information  
Month-Day/Processed : 08/18/21  
Time Processed : 9:04:52  
Injection Volume : 0.2  
Sample Name : Cys-TAT(47-57)  
Cat No. : RP20343  
Lot No. : E9348521H  
Theoretical MW : 1661.99  
Observed MW : 1662.0

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +3.5 kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2 ml/min  
B.conc : 50%H2O/50%MeOH