

Sample Name:C-Peptide (3-33), human
 Cat No.: RP11116
 Lot No.: E7499420A
 Time Processed :15:12:22
 Month-Day-Year Processed :01/09/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

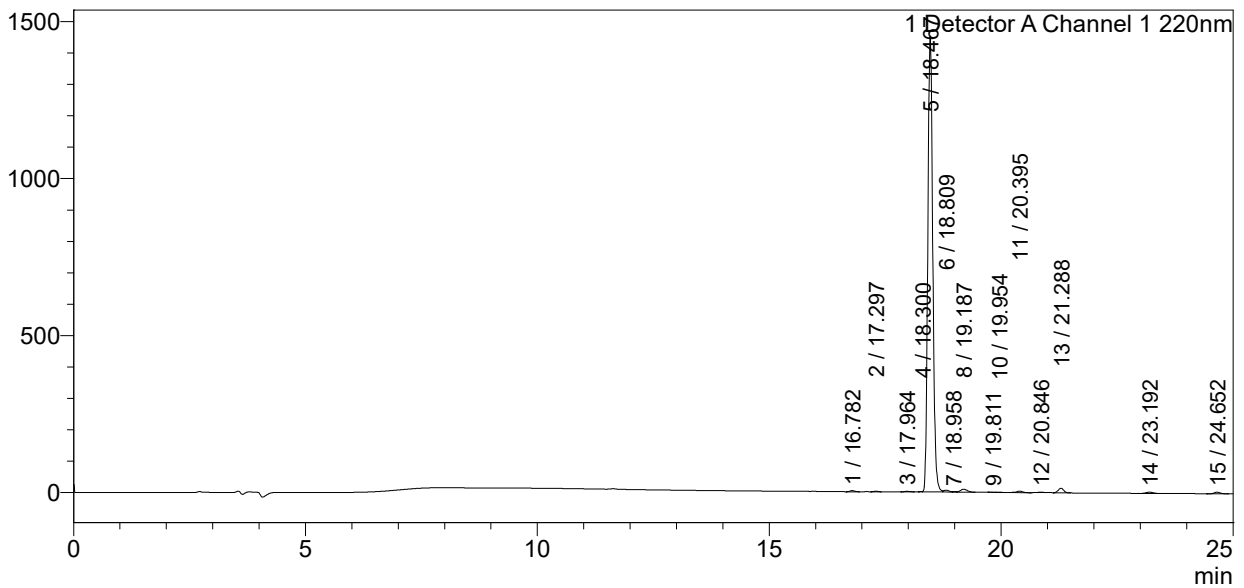

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.782	23449	3595	0.209
2	17.297	10053	1725	0.090
3	17.964	14813	1795	0.132
4	18.300	4082	1093	0.036
5	18.467	10747718	1451419	95.831
6	18.809	46848	5714	0.418
7	18.958	7287	1303	0.065
8	19.187	92153	9088	0.822
9	19.811	6703	1125	0.060
10	19.954	8638	1377	0.077
11	20.395	43224	4873	0.385
12	20.846	10182	1266	0.091
13	21.288	117628	14638	1.049
14	23.192	40584	3993	0.362
15	24.652	41897	4925	0.374

Peak#	Ret. Time	Area	Height	Area%
Total		11215257	1507930	100.000