


Mass Spectrum

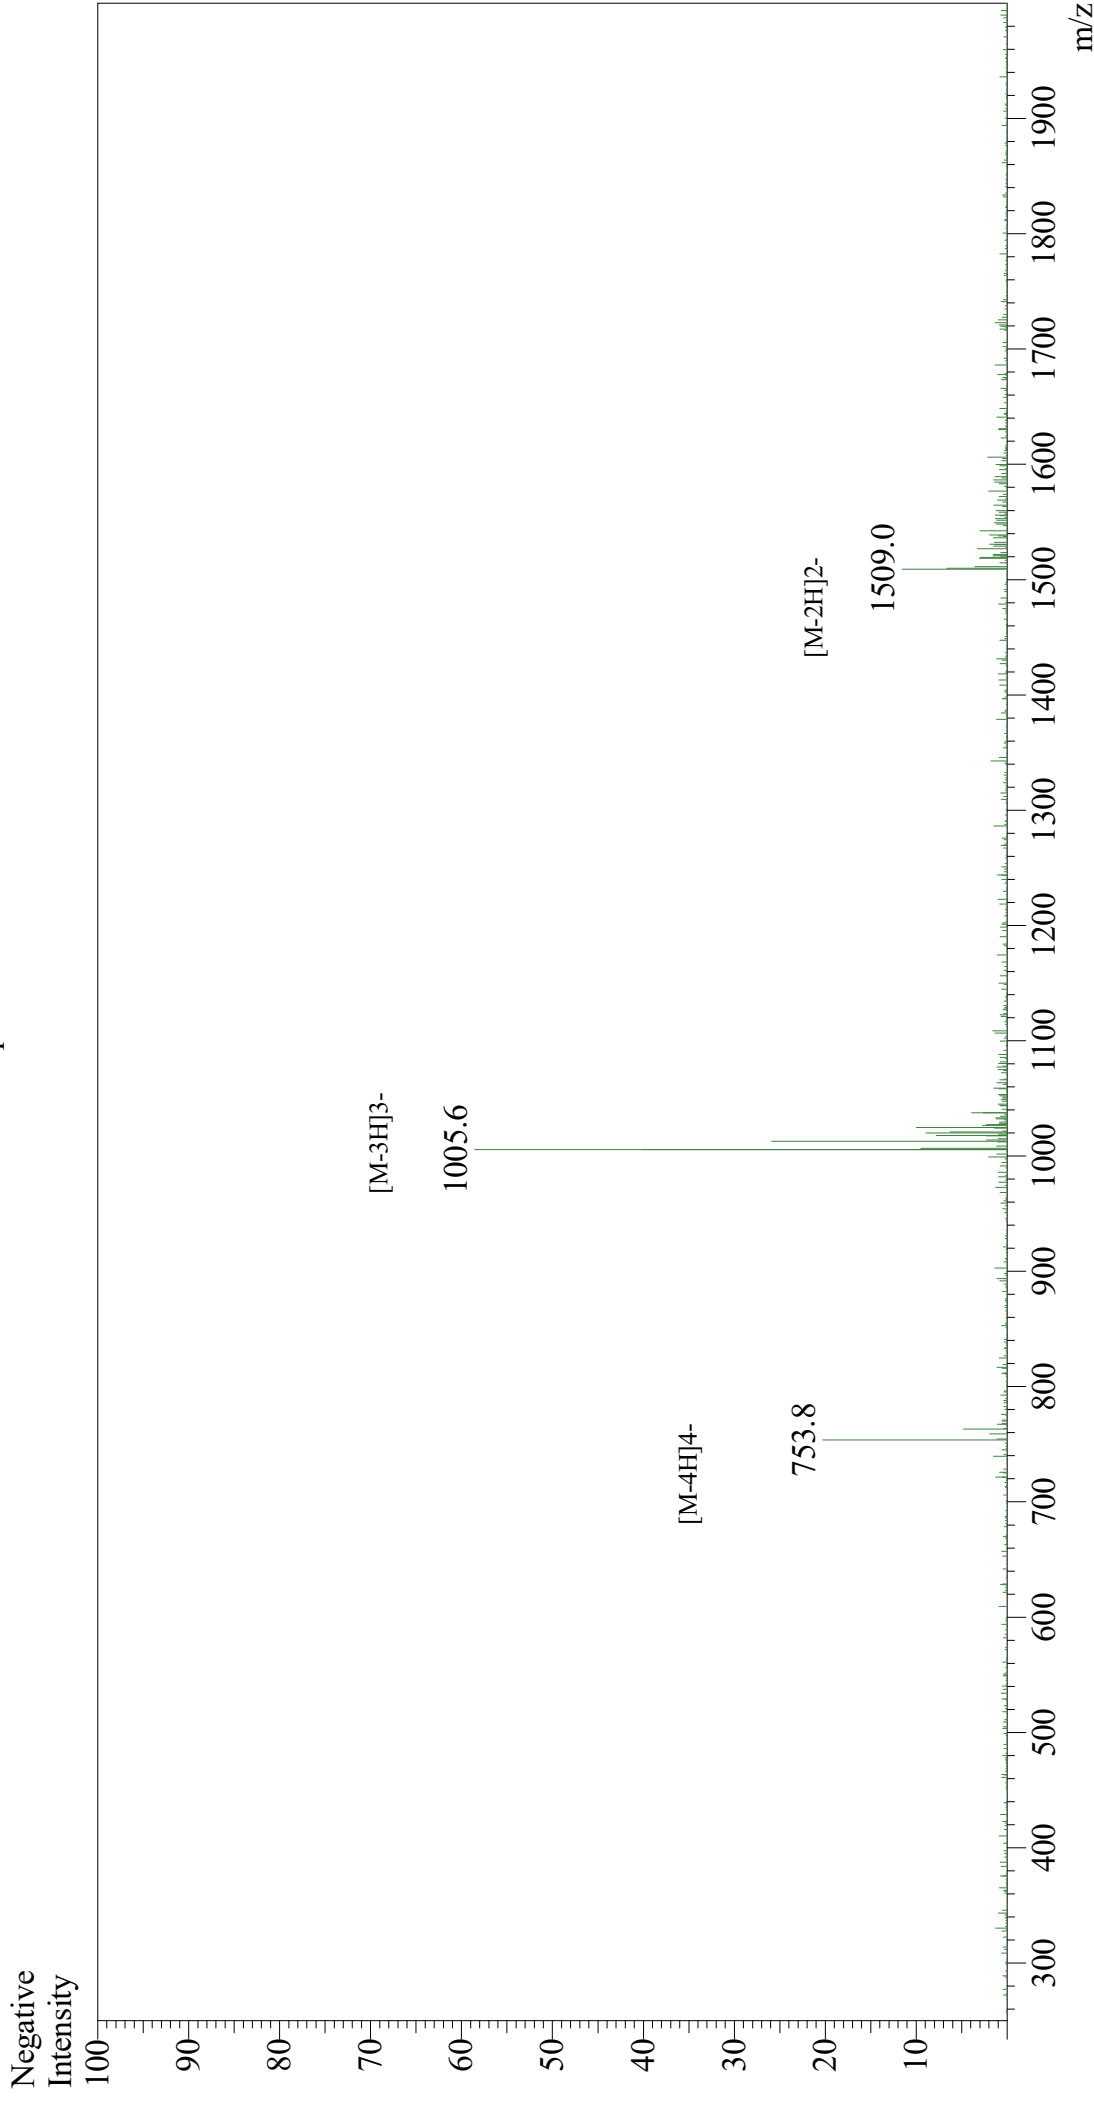

Sample Information

User : Gary
Month-Day Processed : 01/07/20
Time Processed : 03:55:07 PM
Injection Volume : 0.3
Sample Name : C-Peptide (3-33), human
Cat No. : RP11116
Lot No. : E7499420A
Theoretical MW : 3020.26
Observed MW : 3019.8

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : GK11010007
Interface Bias : -3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH