

Sample Name : Transdermal Peptide
 Cat No. : RP20404 Lot No. : PE8021810
 Time Processed : 8:39:44
 Month-Day-Year Processed : 10/30/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	0	
5.00	Pumps	Pump A B.Conc	0	
20.00	Pumps	Pump A B.Conc	30	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	0	
40.00	Pumps	Pump A B.Conc	0	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

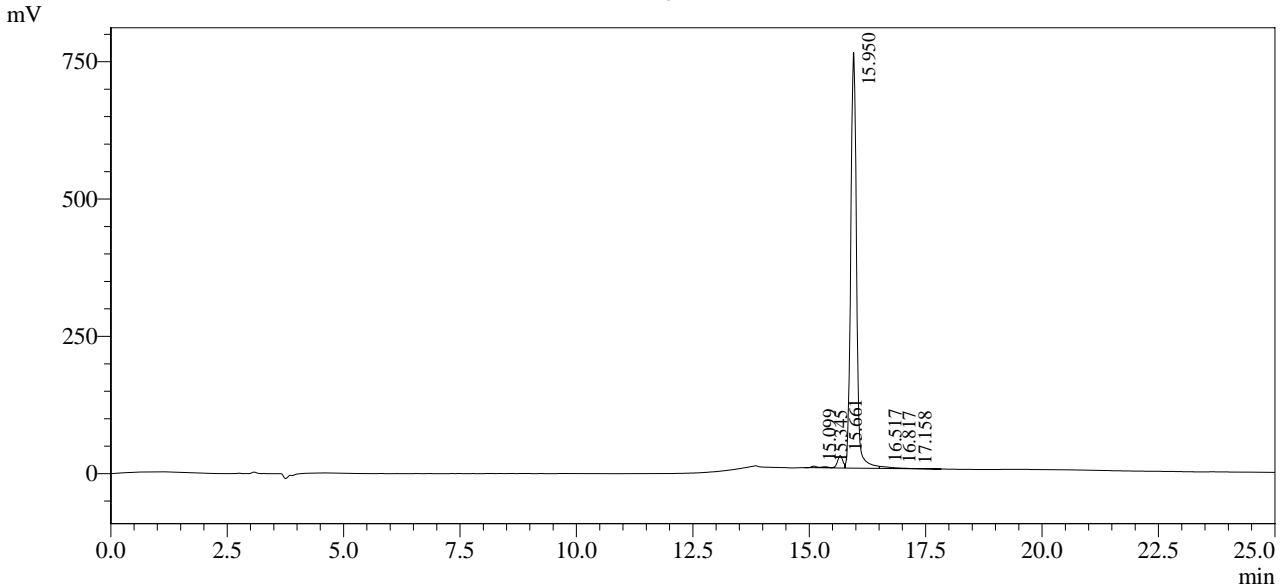

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.099	24114	2860	0.352
2	15.345	18264	2087	0.267
3	15.661	181355	22541	2.650
4	15.950	6544918	756574	95.619
5	16.517	47865	3648	0.699
6	16.817	20158	1436	0.295
7	17.158	8089	507	0.118
Total		6844763	789654	100.000