

Sample Name : Gly-Arg-Gly-Asp-Ser
 Cat. No. : RP10848
 Lot. No. : E7105521A
 Time Processed : 5:18:47 PM
 Month-Day-Year Processed : 01/16/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	0
5.00	Pumps	Pump A B.Conc	0
20.00	Pumps	Pump A B.Conc	30
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	0
35.00	Pumps	Pump A B.Conc	0
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment : SS-CM-0286

<Chromatogram>

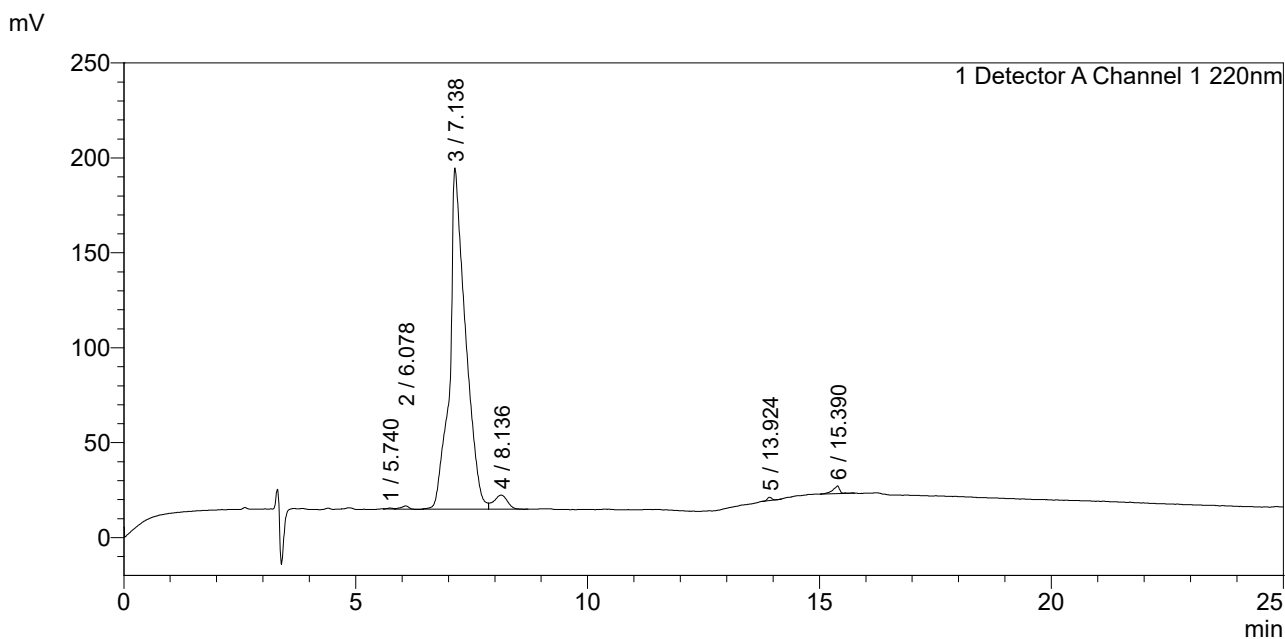

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.740	4308	510	0.096
2	6.078	15542	1687	0.345
3	7.138	4281706	179715	95.085
4	8.136	150009	7393	3.331
5	13.924	10166	1676	0.226
6	15.390	41322	4013	0.918
Total		4503054	194995	100.000