

Sample Name :HPV16 E7(86-93)  
 Cat No.: RP20499  
 Lot No.: E3463319L  
 Time Processed :17:23:41  
 Month-Day-Year Processed :12/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

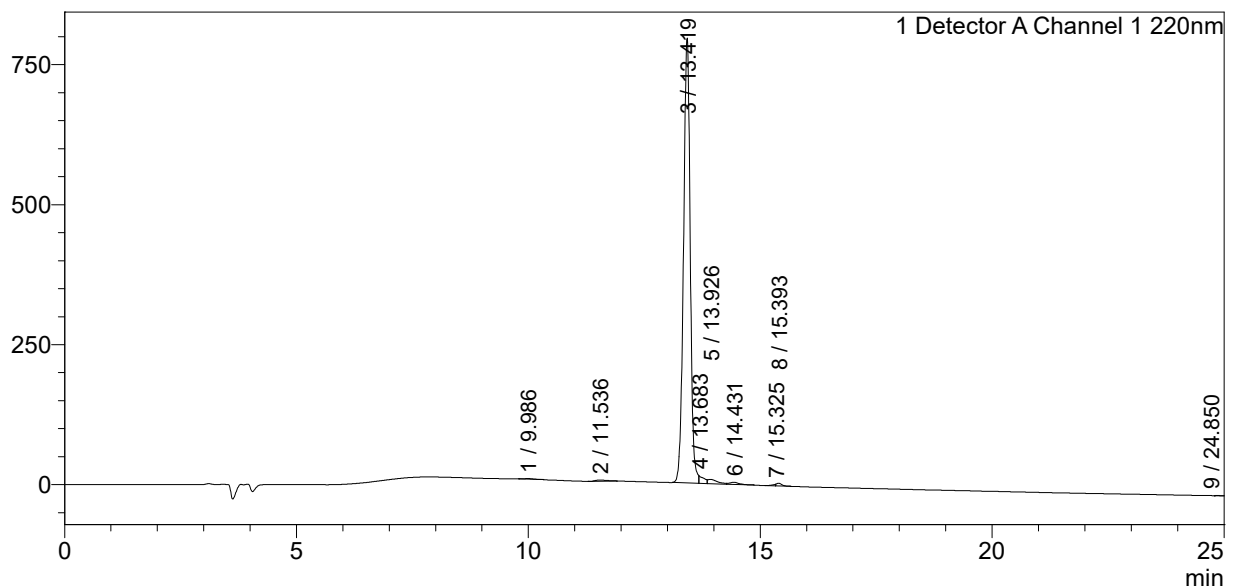

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.986	10794	1005	0.130
2	11.536	36748	2143	0.441
3	13.419	7962132	794883	95.557
4	13.683	104855	13050	1.258
5	13.926	109871	7573	1.319
6	14.431	53382	3946	0.641
7	15.325	15010	2674	0.180
8	15.393	37856	4964	0.454
9	24.850	1677	236	0.020
Total		8332324	830474	100.000