

Sample Name: MOG(35-55)
 Cat No. : RP10245
 Lot No. : E5820520E
 Time Processed: 2:02:34 PM
 Month-Day-Year Processed :05/27/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

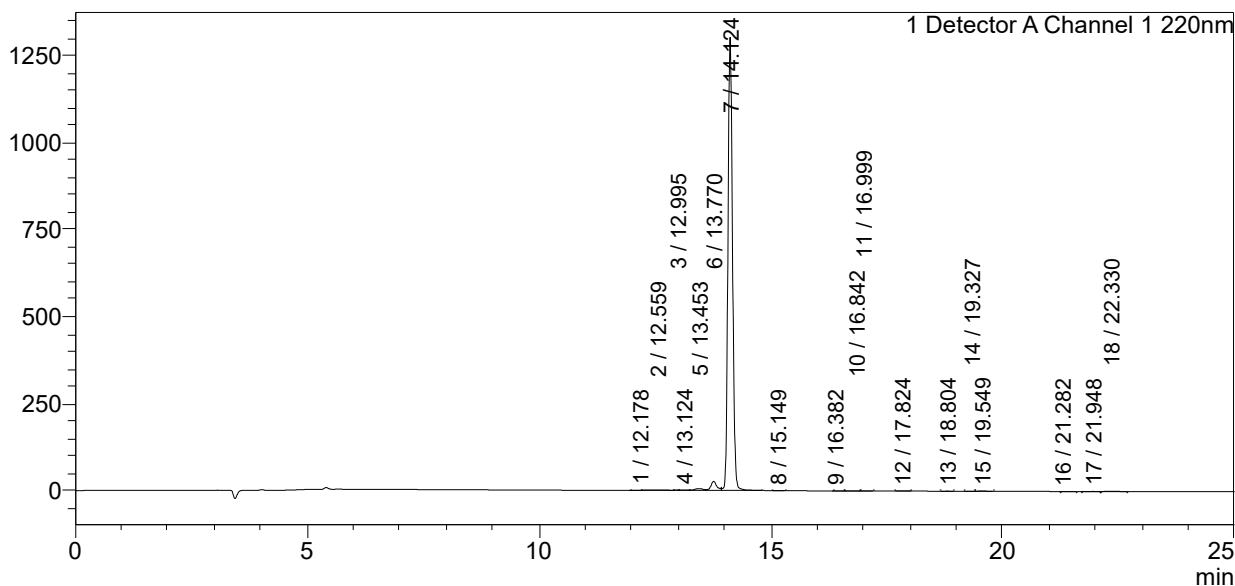

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.178	3266	334	0.035
2	12.559	33709	1176	0.363
3	12.995	6153	875	0.066
4	13.124	12307	1200	0.133
5	13.453	66828	4866	0.720
6	13.770	239270	26317	2.577
7	14.124	8881592	1302794	95.651
8	15.149	2792	424	0.030
9	16.382	1170	115	0.013
10	16.842	2508	246	0.027
11	16.999	3539	431	0.038
12	17.824	1374	148	0.015
13	18.804	1132	149	0.012
14	19.327	1226	139	0.013

Peak#	Ret. Time	Area	Height	Area%
15	19.549	10041	988	0.108
16	21.282	1782	154	0.019
17	21.948	3909	316	0.042
18	22.330	12823	604	0.138
Total		9285419	1341276	100.000