


Mass Spectrum

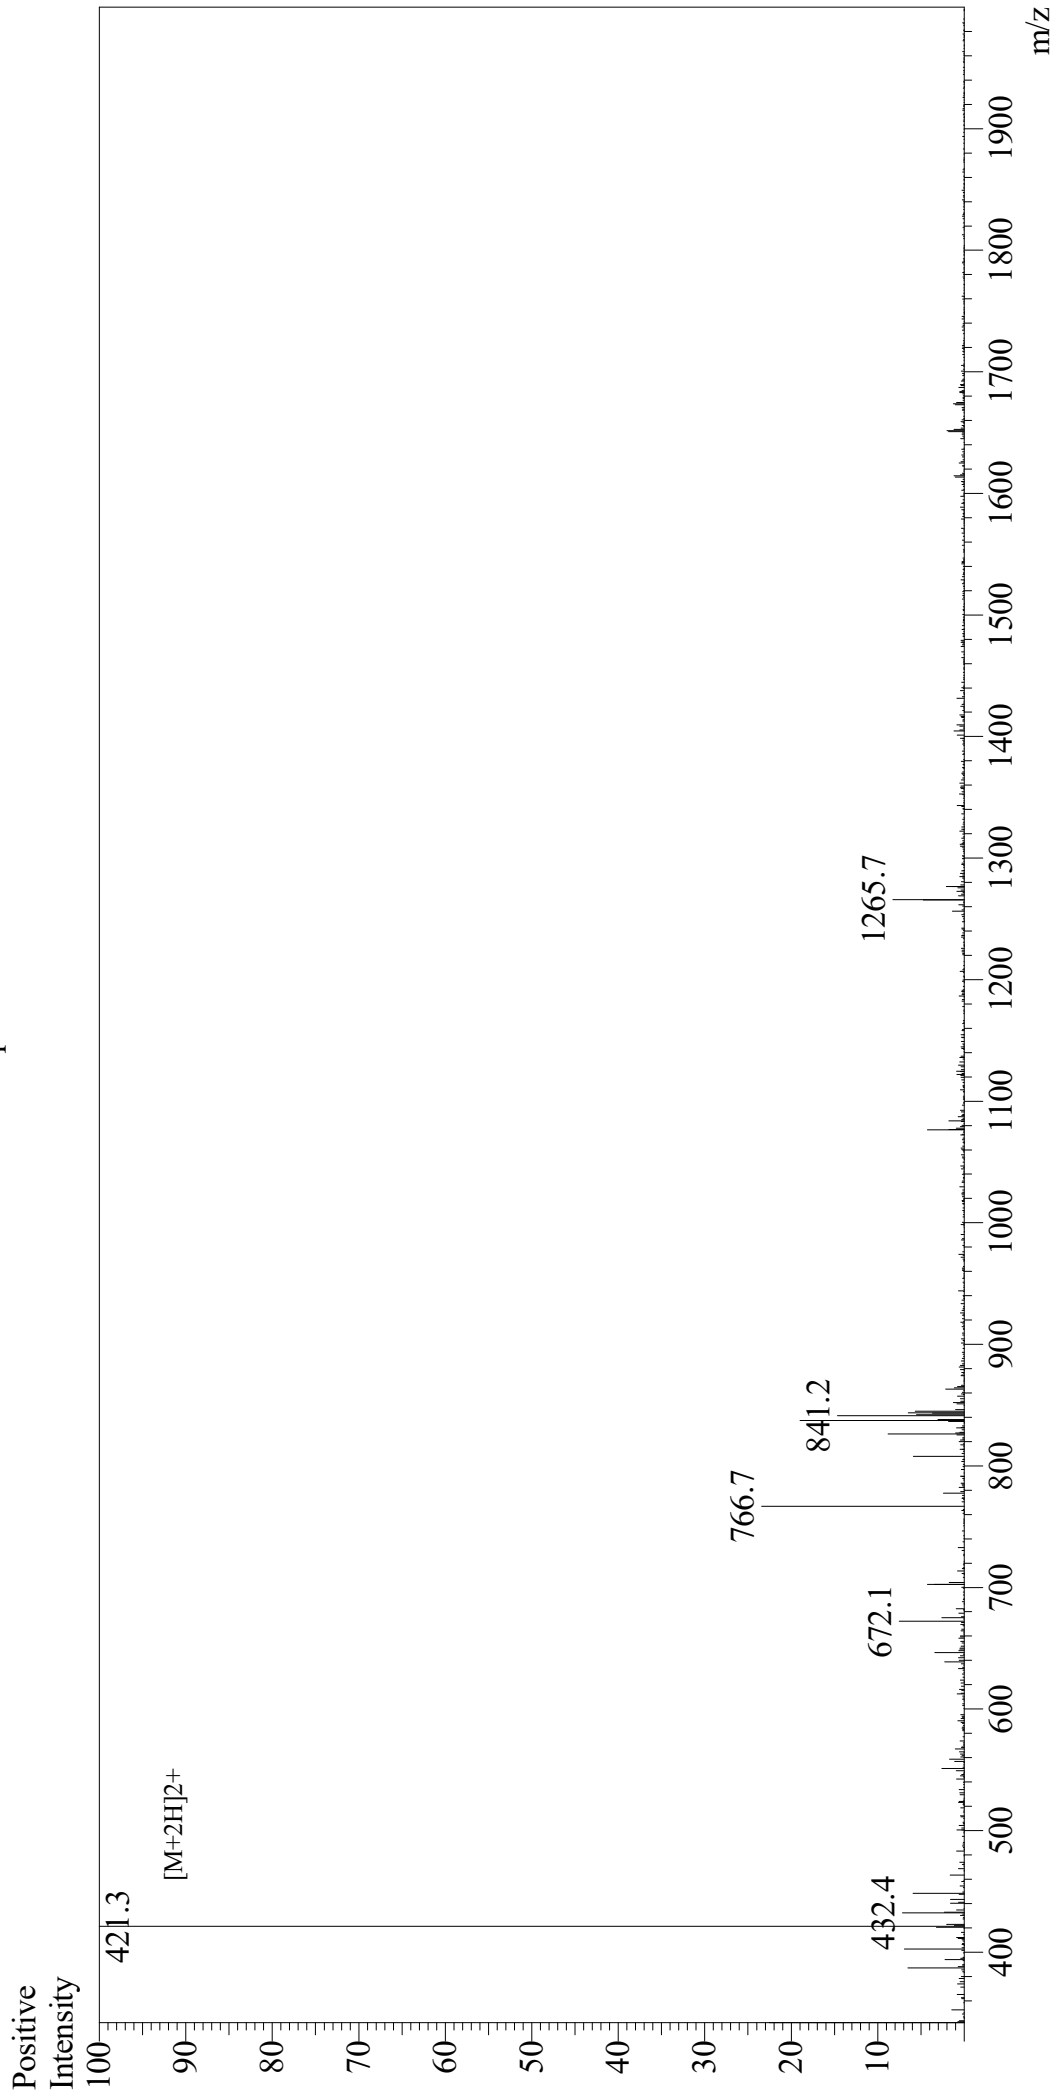

Sample Information

User : Gary
Month-Day Processed : 05/22/20
Time Processed : 09:20:16 AM
Injection Volume : 0.4
Sample Name : Hexa-His
Cat No. : RP11737
Lot No. : E5420520E
Theoretical MW : 840.85
Observed MW : 840.6

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH