

Sample Name :RGD
 Cat. No. : RP20297
 Lot. No. : E3923419F
 Time Processed :8:53:15
 Month-Day-Year Processed :06/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

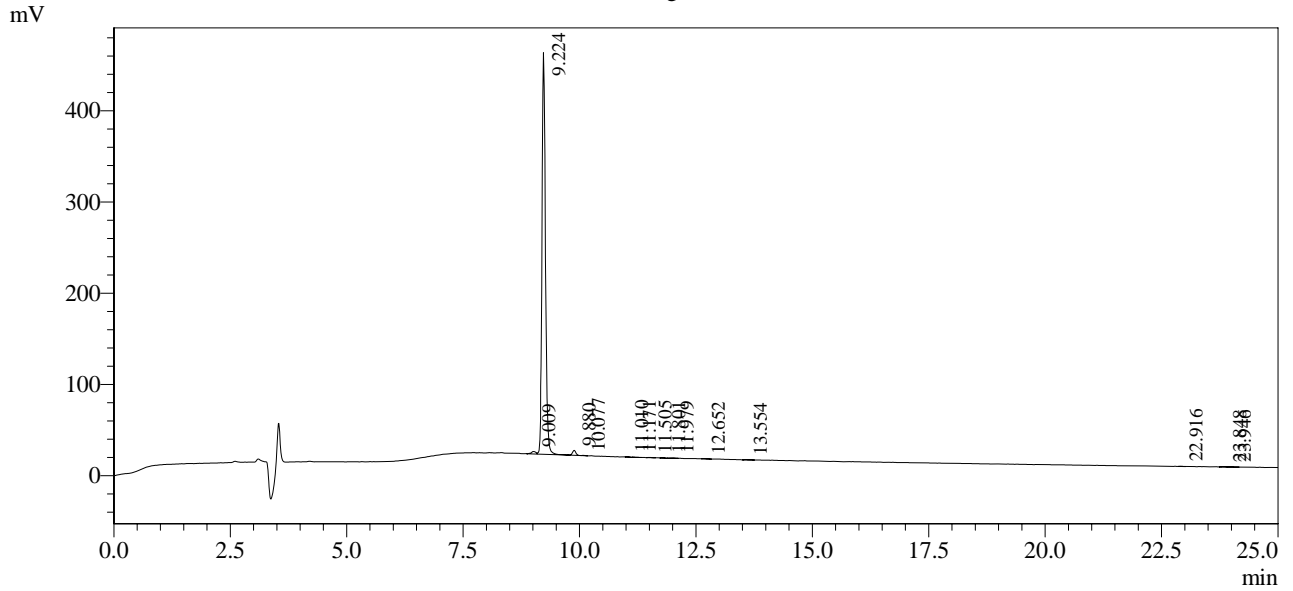

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.009	18815	2682	0.799
2	9.224	2294111	440173	97.376
3	9.880	27429	5418	1.164
4	10.077	1180	316	0.050
5	11.010	1062	144	0.045
6	11.171	1025	187	0.043
7	11.505	1683	330	0.071
8	11.801	1260	259	0.053
9	11.979	2201	268	0.093
10	12.652	1402	186	0.059
11	13.554	1497	175	0.064
12	22.916	1061	265	0.045
13	23.848	1809	274	0.077
14	23.946	1388	170	0.059
Total		2355922	450848	100.000