

Sample Name :43Gap 26, Connexin Mimetic
 Cat No. :RP20274
 Lot No. :E3814619K
 Time Processed :8:45:38 AM
 Month-Day-Year Processed :11/26/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010508

<Chromatogram>

mV

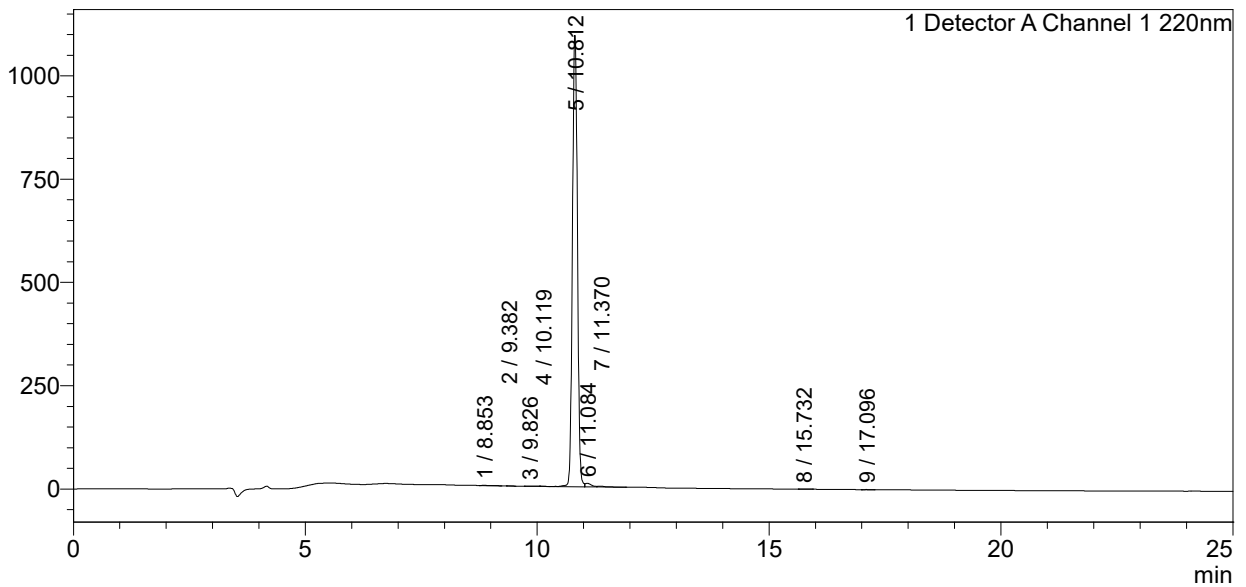

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.853	5908	341	0.071
2	9.382	1363	192	0.016
3	9.826	1462	155	0.018
4	10.119	1343	225	0.016
5	10.812	8222892	1092545	98.690
6	11.084	77492	8418	0.930
7	11.370	18376	2028	0.221
8	15.732	1534	127	0.018
9	17.096	1705	225	0.020
Total		8332074	1104256	100.000