

Sample Name :AngiotensinII,human  
 Cat No. :RP11257  
 Lot No. :E9697719G  
 Time Processed :17:24:32  
 Month-Day-Year Processed :07/21/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ17010508

### <Chromatogram>

mV

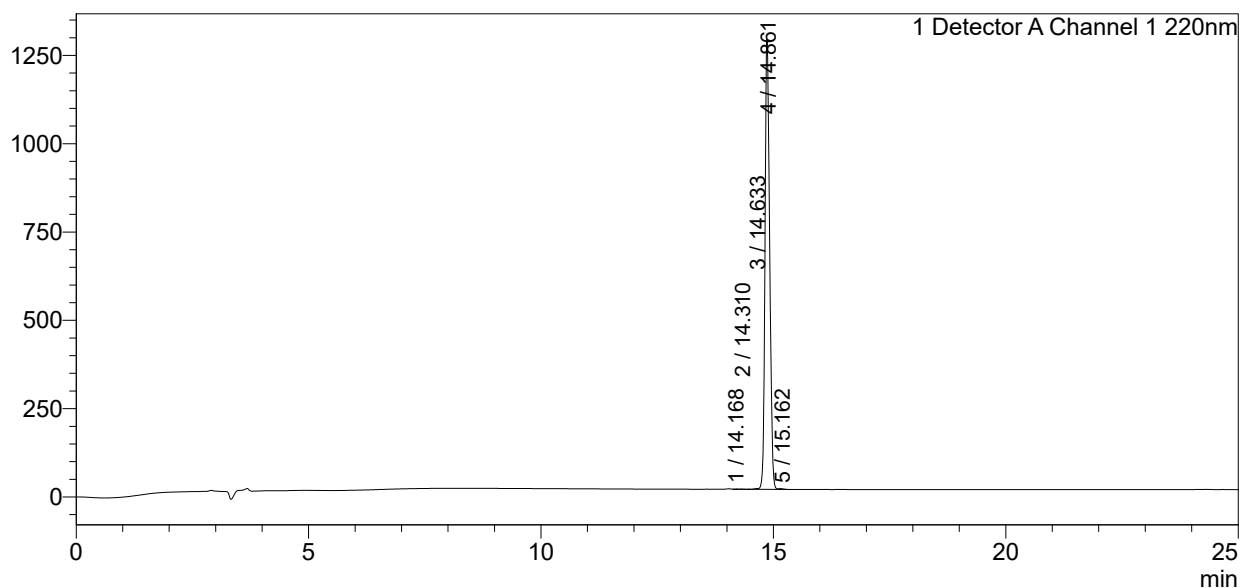

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.168	1525	353	0.017
2	14.310	5059	656	0.057
3	14.633	11476	2130	0.129
4	14.861	8850286	1273640	99.766
5	15.162	2697	696	0.030
Total		8871044	1277476	100.000