

Sample Name: Influenza NP (147-155)  
 Cat No. : RP20260  
 Lot No. : E4874919I  
 Time Processed: 9:16:12 AM  
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment: ZJ19010325

### <Chromatogram>

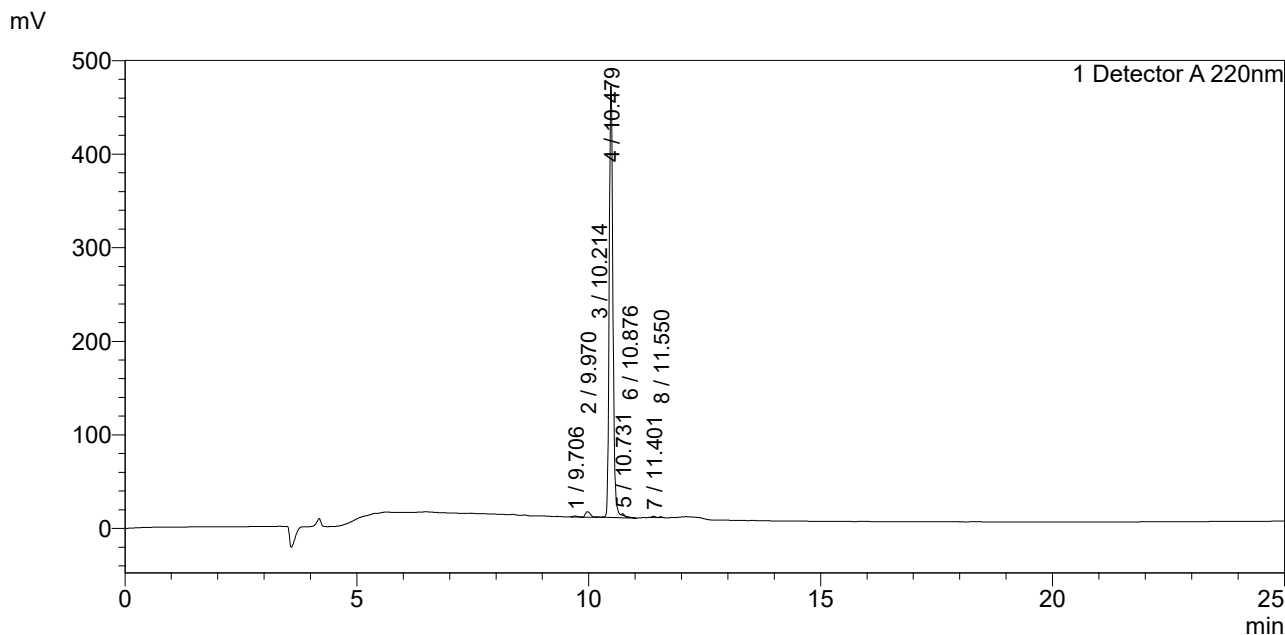

### <Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.706	6670	1164	0.253
2	9.970	43411	5798	1.647
3	10.214	1363	286	0.052
4	10.479	2568589	460955	97.466
5	10.731	5680	1633	0.216
6	10.876	1213	305	0.046
7	11.401	5225	1273	0.198
8	11.550	3229	860	0.123
Total		2635380	472274	100.000