

Sample Name: Gastrin-1, human
 Cat No. :RP12740
 Lot No. :E6819620H
 Time Processed: 11:09:35 AM
 Month-Day-Year Processed :03/12/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
35.00	Pumps	Solvent B Conc.	95
35.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
41.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

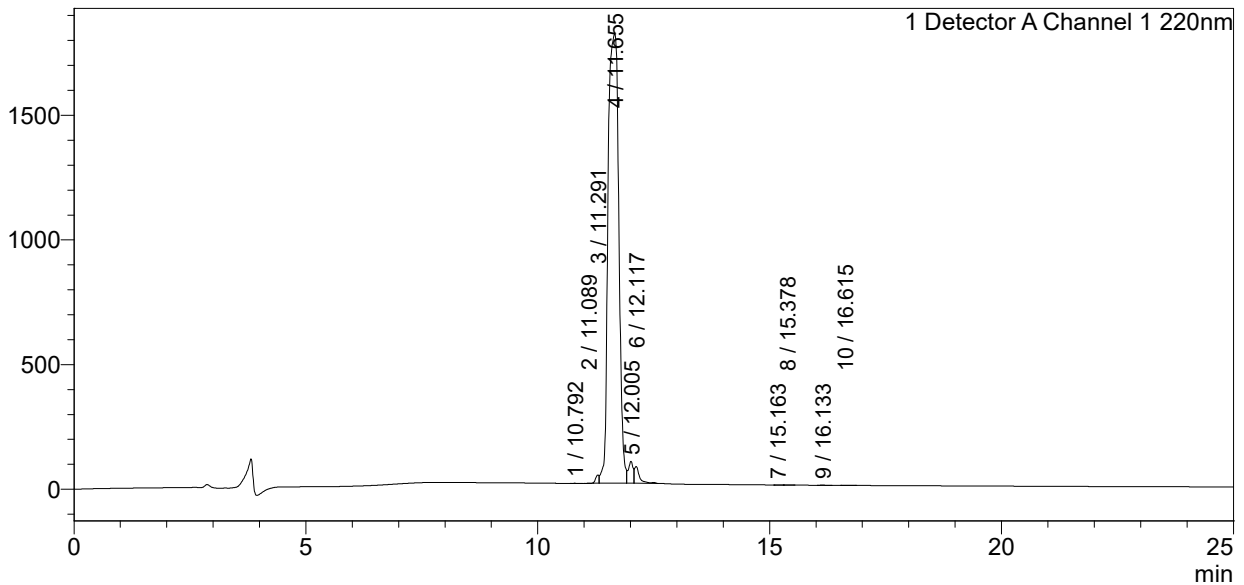

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.792	5783	987	0.019
2	11.089	3429	686	0.011
3	11.291	168083	32555	0.557
4	11.655	28866722	1800915	95.584
5	12.005	640103	88192	2.120
6	12.117	505563	67003	1.674
7	15.163	1545	251	0.005
8	15.378	2254	434	0.007
9	16.133	3883	616	0.013
10	16.615	2973	451	0.010
Total		30200339	1992091	100.000