

Sample Name :Angiotensin II, human
 Cat No. :RP11257
 Lot No. :PE5901903

Time Processed : 13:19:37
 Month-Day-Year Processed : 03/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|--------------|-------|
| 0.01 | Pumps | Pump B Conc. | 5 |
| 25.00 | Pumps | Pump B Conc. | 65 |
| 25.01 | Pumps | Pump B Conc. | 95 |
| 27.00 | Pumps | Pump B Conc. | 95 |
| 27.01 | Pumps | Pump B Conc. | 5 |
| 32.00 | Pumps | Pump B Conc. | 5 |
| 32.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

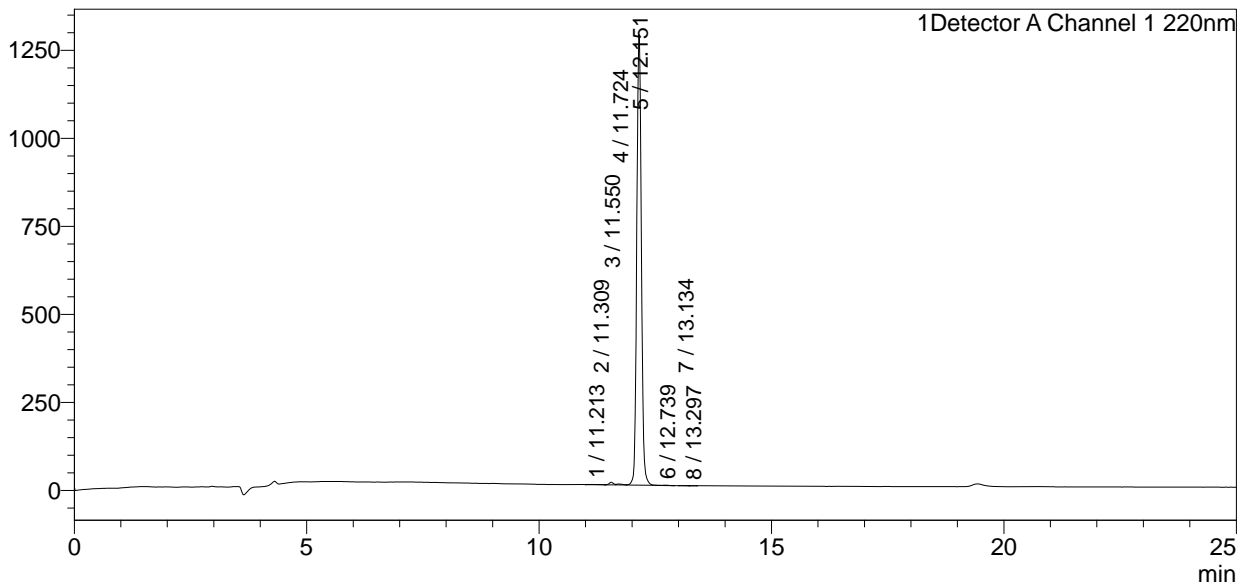

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|---------|---------|
| 1 | 11.213 | 8316 | 992 | 0.093 |
| 2 | 11.309 | 3767 | 792 | 0.042 |
| 3 | 11.550 | 46442 | 7277 | 0.522 |
| 4 | 11.724 | 25815 | 3051 | 0.290 |
| 5 | 12.151 | 8806797 | 1278836 | 98.915 |
| 6 | 12.739 | 9051 | 1007 | 0.102 |
| 7 | 13.134 | 2023 | 297 | 0.023 |
| 8 | 13.297 | 1147 | 221 | 0.013 |
| Total | | 8903359 | 1292473 | 100.000 |