

Sample Name :Kemptide
Cat. No. : RP10287
Lot. No. : PE6141903
Time Processed : 8:19:12
Month-Day-Year Processed : 03/06/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

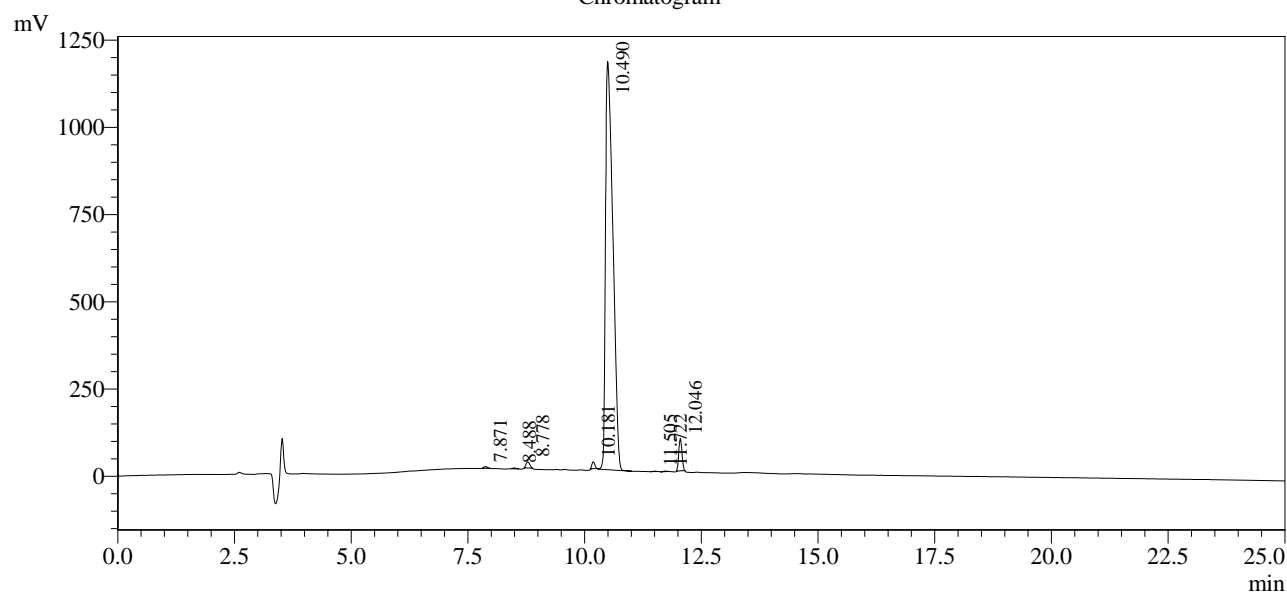

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.871	24287	5048	0.179
2	8.488	9874	2145	0.073
3	8.778	95731	17305	0.706
4	10.181	87415	20112	0.645
5	10.490	12879511	1170883	95.022
6	11.505	5443	1287	0.040
7	11.722	8463	1892	0.062
8	12.046	443496	92760	3.272
Total		13554219	1311432	100.000