

Sample Name : Proctolin
 Cat. No. : RP10475
 Lot. No. : PE3981812
 Time Processed : 1:21:57
 Month-Day-Year Processed : 12/19/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

Chromatogram

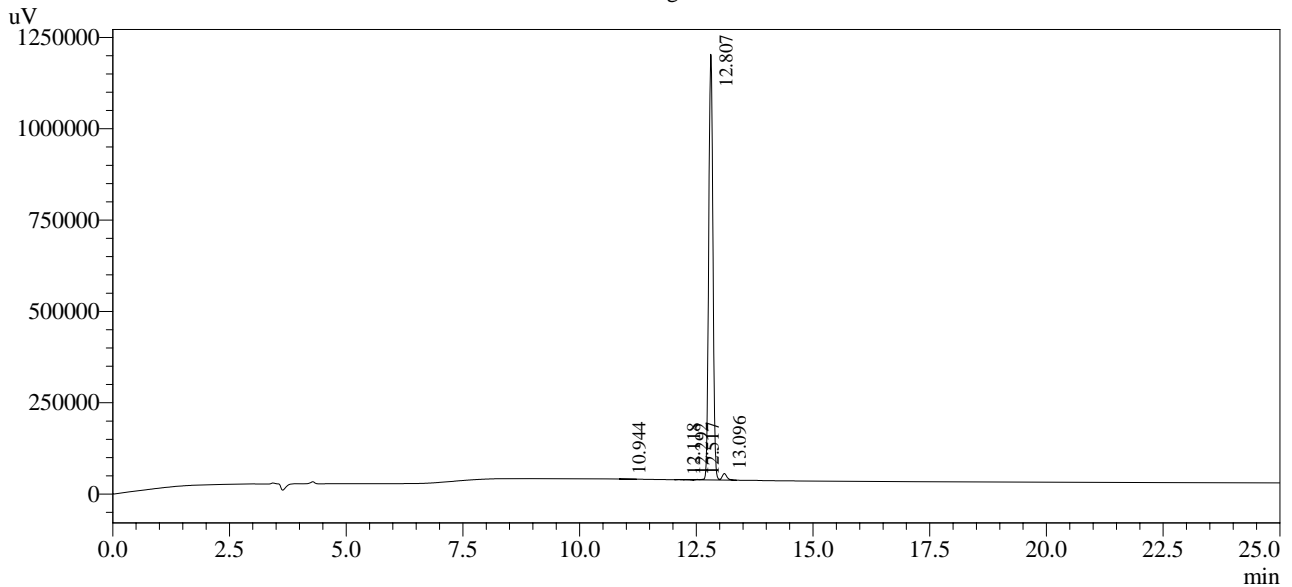

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.944	4080	577	0.055
2	12.118	2245	443	0.030
3	12.292	1722	311	0.023
4	12.517	6152	1169	0.082
5	12.807	7336948	1165278	98.115
6	13.096	126784	18072	1.695
Total		7477931	1185850	100.000