

Sample Name :GroES mobile loop
 Cat. No. :RP20179
 Lot. No. :E4830319I
 Time Processed :13:33:19
 Month-Day-Year Processed :09/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

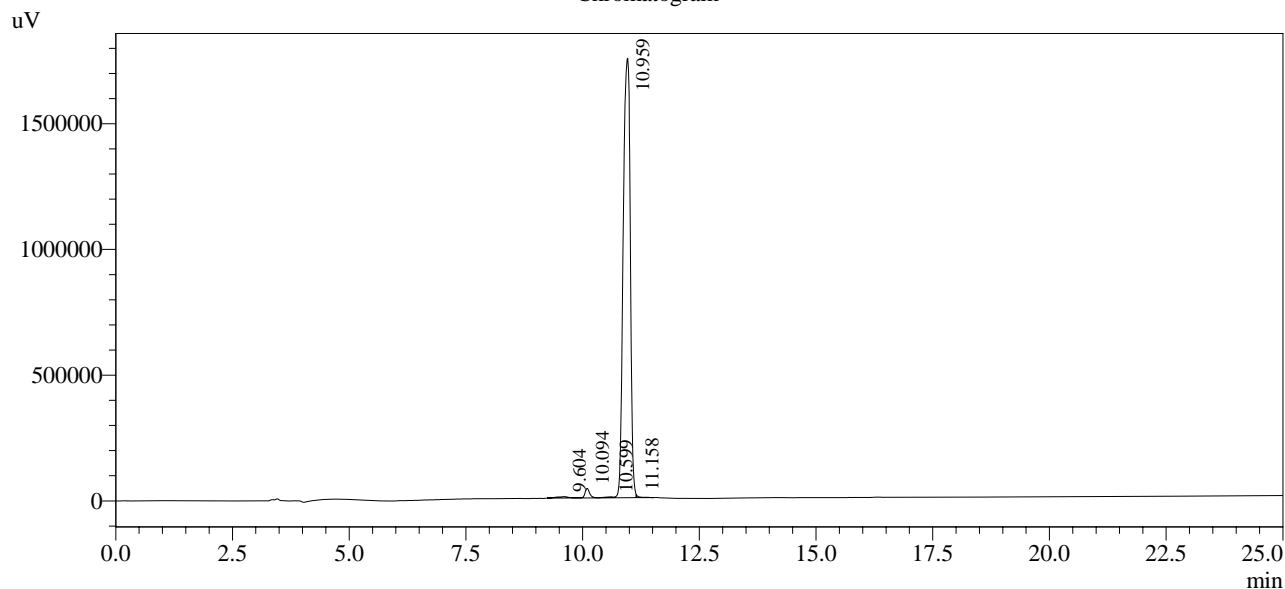

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.604	108281	5689	0.574
2	10.094	268327	38334	1.423
3	10.599	55390	3889	0.294
4	10.959	18379844	1747860	97.491
5	11.158	40982	9629	0.217
Total		18852826	1805402	100.000