

Sample Name :Endothelin 1, human, porcine
Cat No.: RP12758
Lot No.: PE8021810
Time Processed:11:18:26
Month-Day-Year Processed:12/11/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

<Chromatogram>

mV

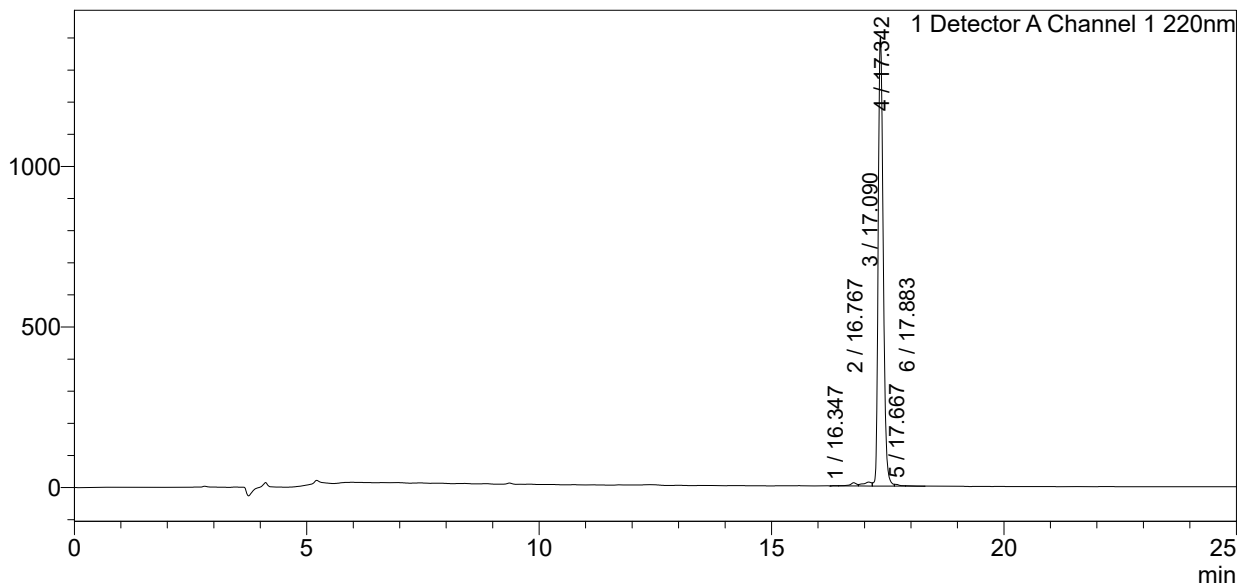

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.347	5637	964	0.052
2	16.767	100189	10245	0.929
3	17.090	154965	12306	1.437
4	17.342	10468423	1401731	97.081
5	17.667	41187	5797	0.382
6	17.883	12811	832	0.119
Total		10783211	1431875	100.000