

Sample Name : (Arg)9
 Cat No. : RP20403
 Lot No. : E9618319L
 Time Processed : 22:25:07
 Month-Day-Year Processed : 12/21/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

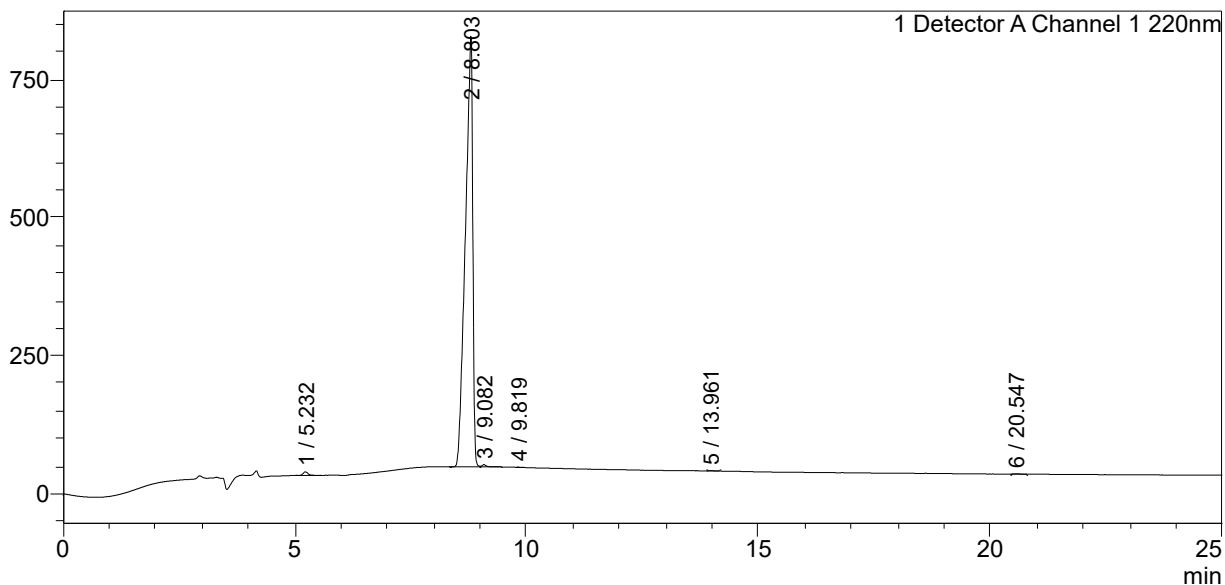

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.232	47663	6508	0.549
2	8.803	8593493	780666	99.006
3	9.082	27318	4137	0.315
4	9.819	1069	294	0.012
5	13.961	3876	512	0.045
6	20.547	6363	791	0.073
Total		8679782	792908	100.000