

Sample Name :N-Formyl-Nle-Leu-Phe-Nle-Tyr-Lys  
 Cat No. : RP12959  
 Lot No. :PE5697419F  
 Time Processed : 22:51:39  
 Month-Day-Year Processed : 06/30/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

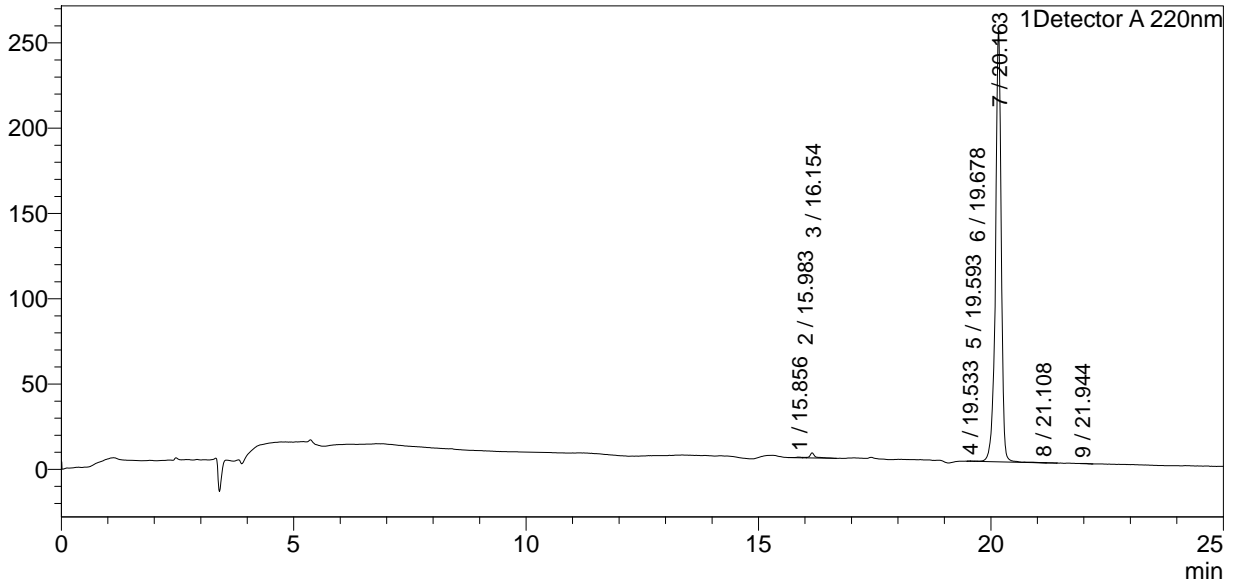

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.856	3273	384	0.150
2	15.983	1297	302	0.059
3	16.154	24555	2994	1.122
4	19.533	350	118	0.016
5	19.593	690	177	0.032
6	19.678	598	176	0.027
7	20.163	2155183	252292	98.486
8	21.108	1086	81	0.050
9	21.944	1278	116	0.058
Total		2188309	256639	100.000