

Sample Name :Gastrin-1, human  
 Cat No. :RP12740  
 Lot No. :E2379820F  
 Time Processed :10:01:46  
 Month-Day-Year Processed :06/13/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

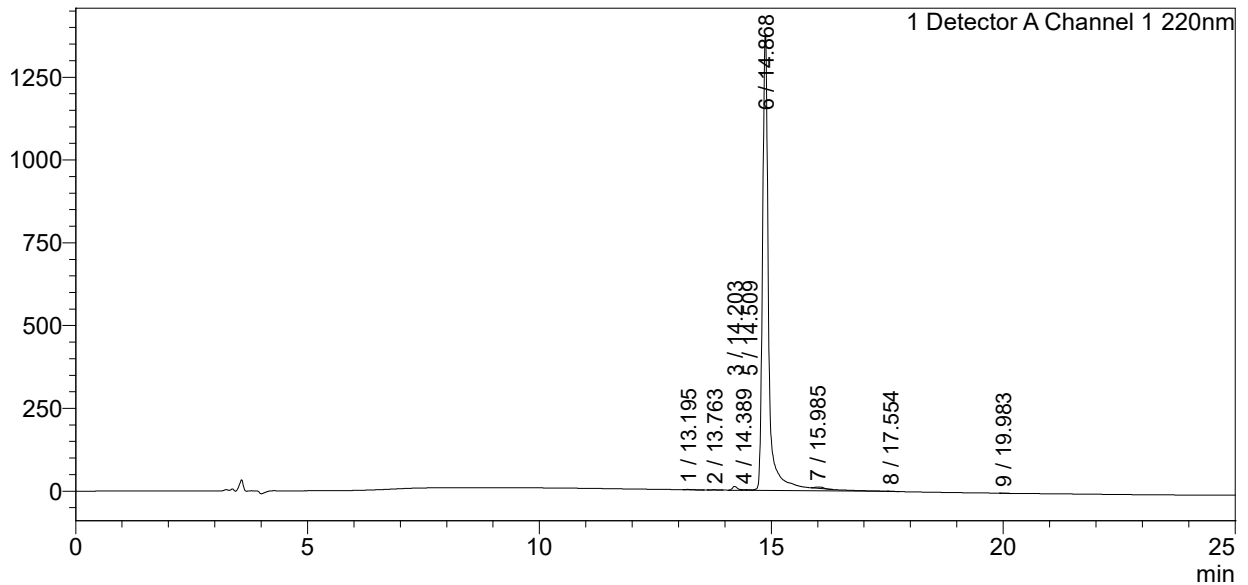

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.195	6685	869	0.051
2	13.763	7741	863	0.059
3	14.203	87750	11498	0.670
4	14.389	11569	1931	0.088
5	14.509	11096	1822	0.085
6	14.868	12915181	1378331	98.623
7	15.985	51828	3761	0.396
8	17.554	2432	232	0.019
9	19.983	1263	155	0.010
Total		13095545	1399460	100.000