

Sample Name :Gastrin-1, human  
 Cat No. :RP12740  
 Lot No. :E4182219F  
 Time Processed :13:15:31  
 Month-Day-Year Processed :06/21/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ17010508

<Chromatogram>

mV

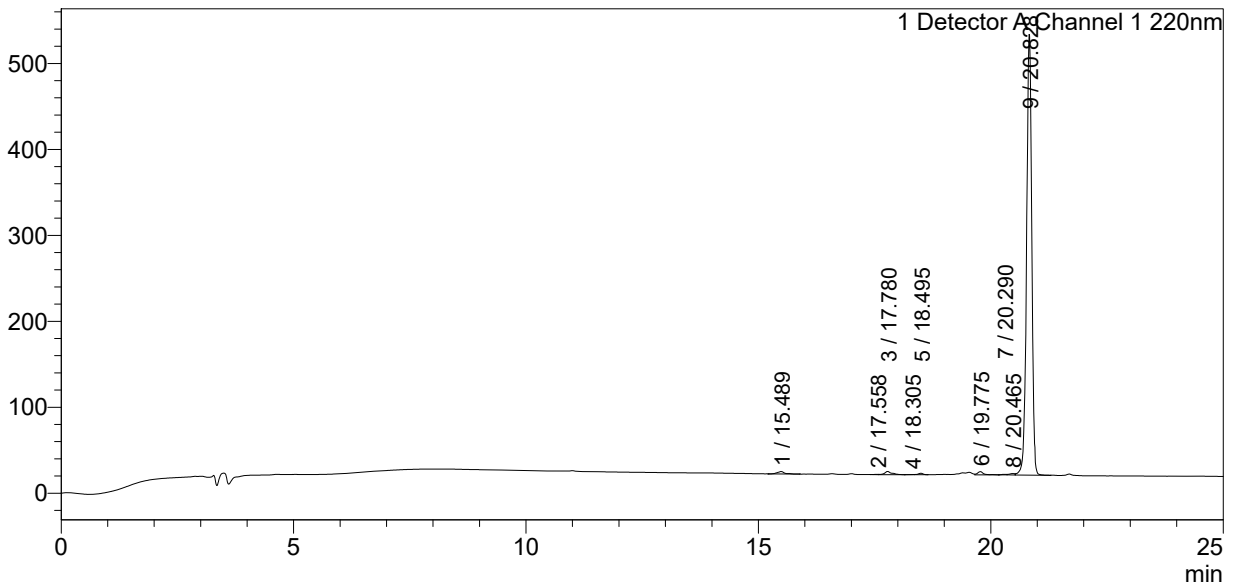

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.489	29840	2788	0.732
2	17.558	1817	272	0.045
3	17.780	40619	3748	0.997
4	18.305	1296	192	0.032
5	18.495	12113	1700	0.297
6	19.775	30711	3710	0.754
7	20.290	4619	640	0.113
8	20.465	12613	1595	0.310
9	20.828	3941183	512676	96.721
Total		4074810	527322	100.000