

Sample Name :Gly-Arg-Gly-Asp-Ser
 Cat. No. : RP10848
 Lot. No. : E4775619I
 Time Processed :10:15:26
 Month-Day-Year Processed : 09/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	0	
5.00	Pumps	Pump A B.Conc	0	
20.00	Pumps	Pump A B.Conc	30	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	0	
40.00	Pumps	Pump A B.Conc	0	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

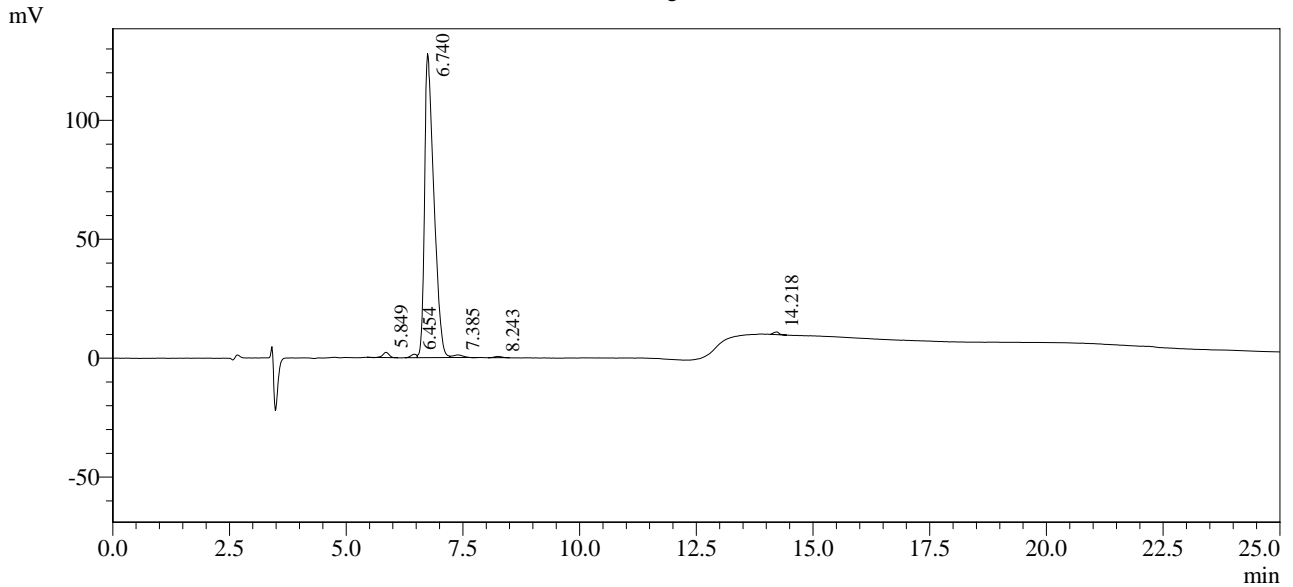

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.849	19991	2205	1.090
2	6.454	12647	1453	0.689
3	6.740	1770880	127867	96.514
4	7.385	16268	1111	0.887
5	8.243	5985	526	0.326
6	14.218	9068	1135	0.494
Total		1834839	134296	100.000