

Sample Name :Dynorphin A(1-13),porcine
Cat. No. : RP20492 Lot. No. : PE3811808
Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

<Chromatogram>

mV

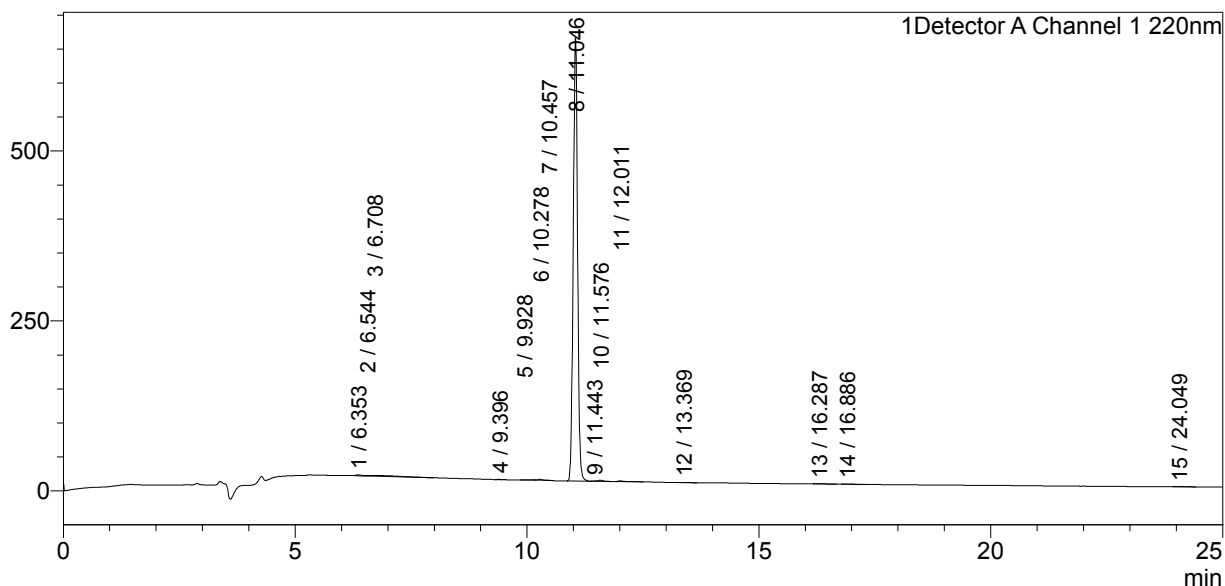

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.353	15064	1372	0.342
2	6.544	11046	1021	0.251
3	6.708	59082	1216	1.343
4	9.396	1881	319	0.043
5	9.928	1125	81	0.026
6	10.278	7310	1298	0.166
7	10.457	1384	297	0.031
8	11.046	4265013	651734	96.944
9	11.443	1609	363	0.037
10	11.576	12319	1778	0.280
11	12.011	10216	1073	0.232
12	13.369	1992	254	0.045
13	16.287	5536	416	0.126
14	16.886	3117	185	0.071
15	24.049	2775	182	0.063
Total		4399470	661590	100.000