

Sample Name :ACTH (1-39), rat  
 Cat No. :RP11305  
 Lot No. :PE5671810  
 Time Processed :9:41:32  
 Month-Day-Year Processed :11/06/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.00	Controller	Stop	

<<Column Performance>>

<Detector A>  
 Column : AlltimaTM C18 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

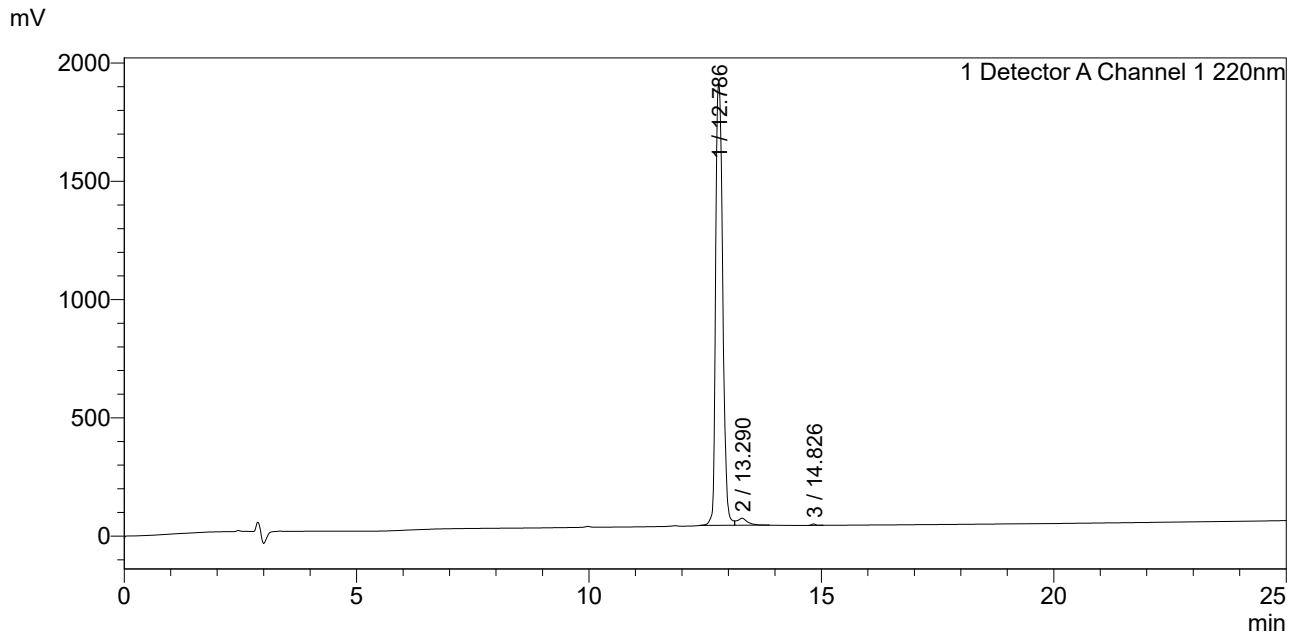

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.786	19722275	1868190	97.487
2	13.290	472424	29948	2.335
3	14.826	36000	6121	0.178
Total		20230699	1904259	100.000