

Sample Name : DYKDDDDK Peptide  
 Cat. No. : RP10586  
 Lot. No. : PE9691707

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

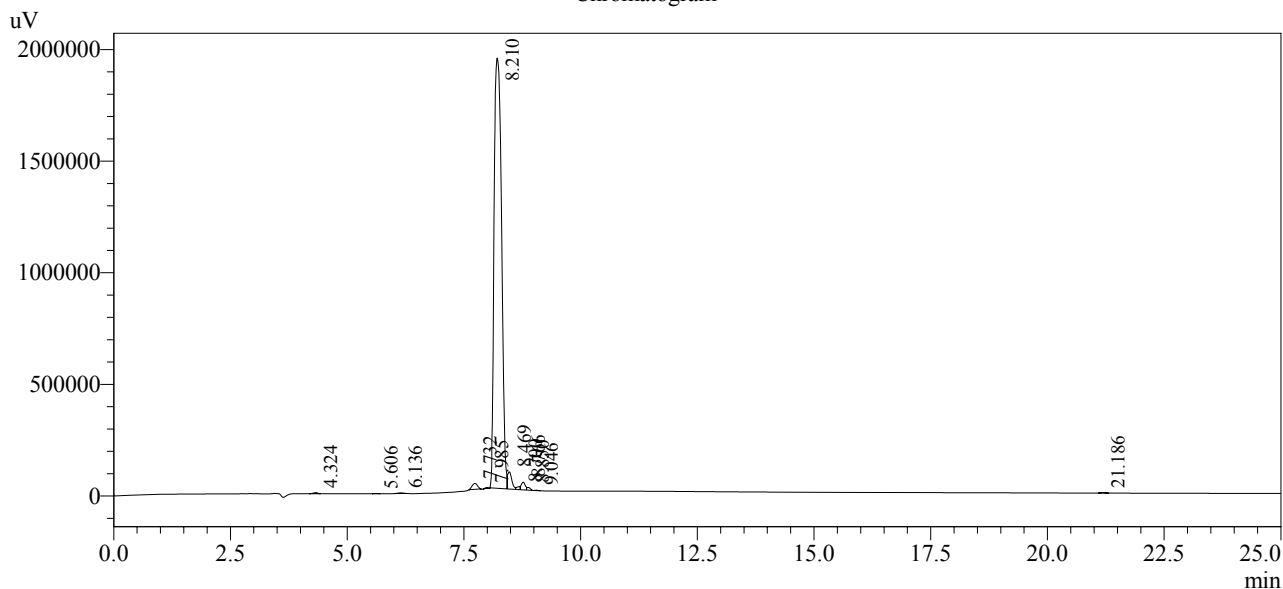

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	4.324	28960	4770	0.129
2	5.606	3801	702	0.017
3	6.136	22399	2701	0.099
4	7.732	214415	26649	0.952
5	7.985	17979	4123	0.080
6	8.210	21409318	1927436	95.078
7	8.469	474620	76703	2.108
8	8.700	69369	13511	0.308
9	8.766	197326	34480	0.876
10	8.850	59962	11454	0.266
11	9.046	7813	1975	0.035
12	21.186	11603	1854	0.052
Total		22517563	2106358	100.000