

Sample Name:[Met5]-Enkephalin  
 Cat No.: RP10886  
 Lot No.: E7940920H  
 Time Processed :22:28:03  
 Month-Day-Year Processed :09/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010014

### <Chromatogram>

mV

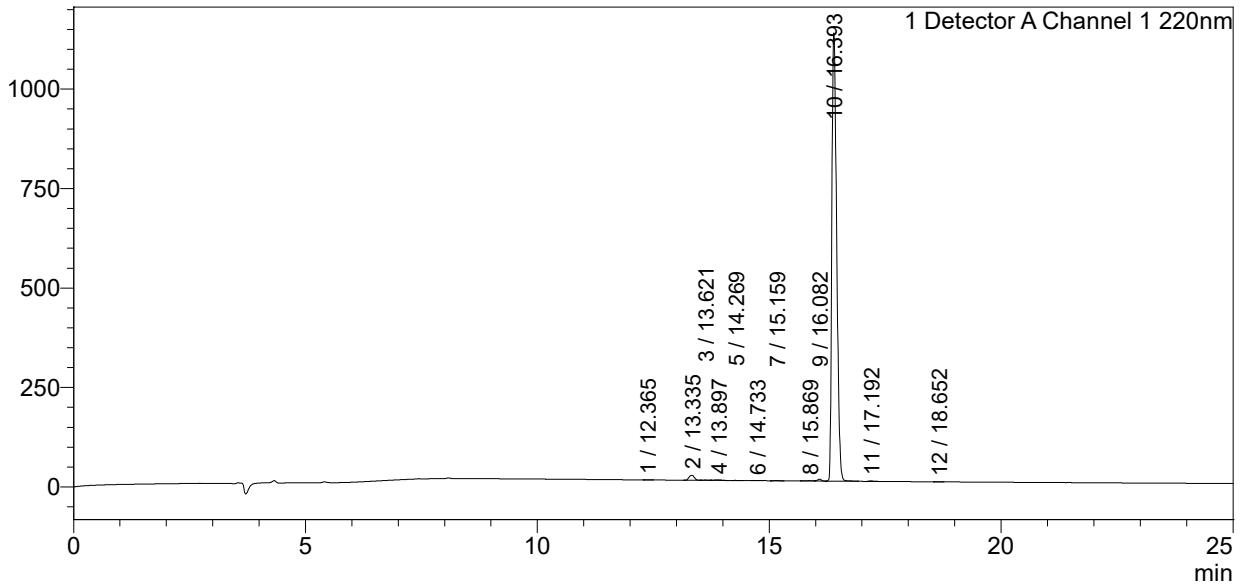

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.365	1733	341	0.021
2	13.335	97257	12202	1.182
3	13.621	2704	487	0.033
4	13.897	12254	1368	0.149
5	14.269	1320	242	0.016
6	14.733	2942	489	0.036
7	15.159	5858	1037	0.071
8	15.869	6041	783	0.073
9	16.082	26800	4817	0.326
10	16.393	8060955	1126978	97.932
11	17.192	12189	1766	0.148
12	18.652	1151	217	0.014
Total		8231204	1150728	100.000