

Sample Name : Gastrin-1, human
 Cat. No. : RP12740
 Lot. No. : E9476120B
 Time Processed : 9:49:13
 Month-Day-Year Processed : 02/20/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

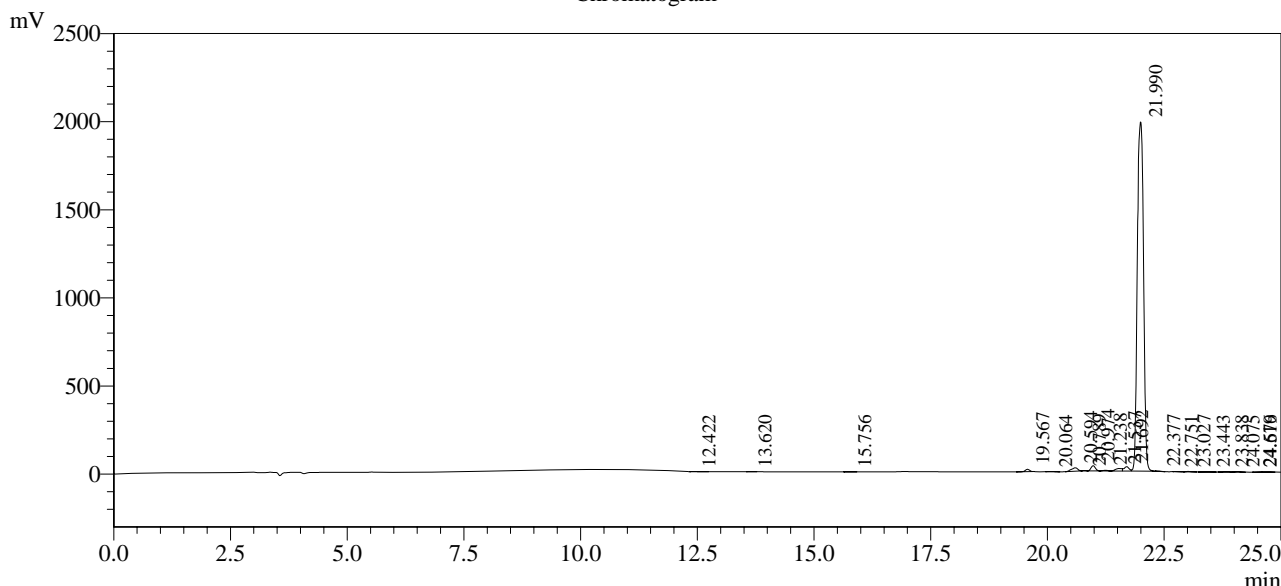

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.422	1690	167	0.009
2	13.620	1395	246	0.007
3	15.756	2960	417	0.015
4	19.567	88631	13746	0.460
5	20.064	12250	1079	0.064
6	20.594	186893	19408	0.971
7	20.789	8294	2054	0.043
8	20.974	190360	29167	0.989
9	21.238	29089	4011	0.151
10	21.537	144353	14709	0.750
11	21.692	186667	25045	0.970
12	21.990	18313335	1981537	95.117
13	22.377	10102	1705	0.052
14	22.751	7222	1076	0.038
15	23.027	19649	2973	0.102
16	23.443	9982	975	0.052
17	23.838	13422	1482	0.070
18	24.075	17076	2558	0.089
19	24.519	2234	470	0.012
20	24.676	7860	1050	0.041
Total		19253464	2103875	100.000