

Sample Name : Ghrelin, rat

Cat. No. : RP10781 Lot. No. : PE7551801

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

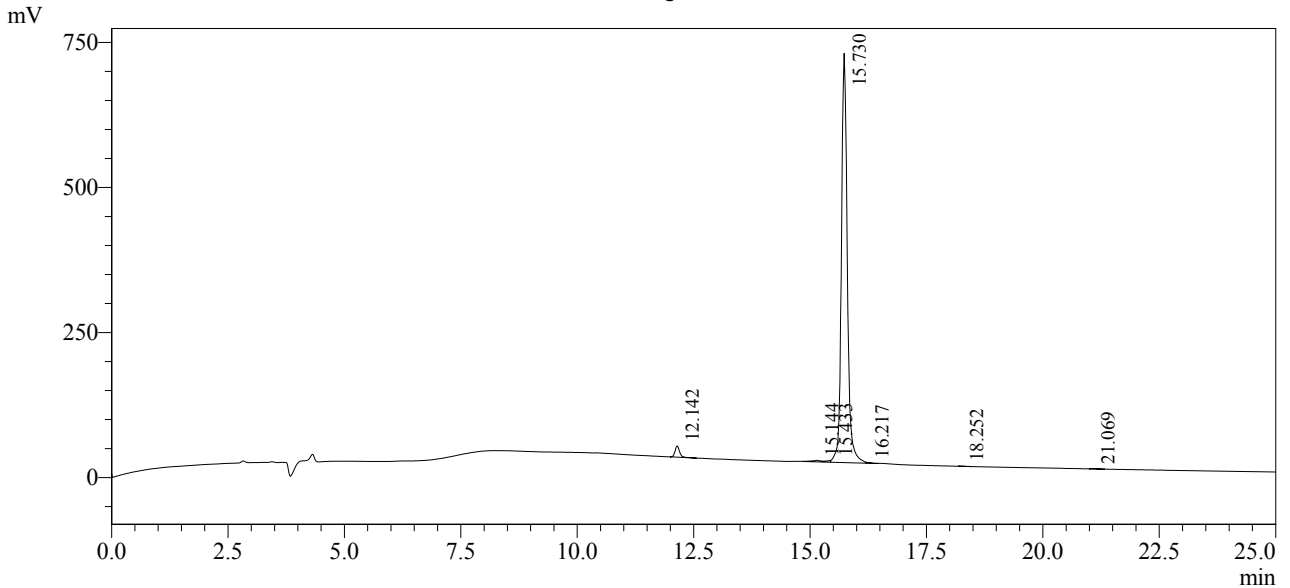

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.142	131847	19134	2.054
2	15.144	36444	2514	0.568
3	15.433	19370	2936	0.302
4	15.730	6217000	705302	96.872
5	16.217	8779	1453	0.137
6	18.252	2144	380	0.033
7	21.069	2185	252	0.034
Total		6417769	731970	100.000