


Mass Spectrum

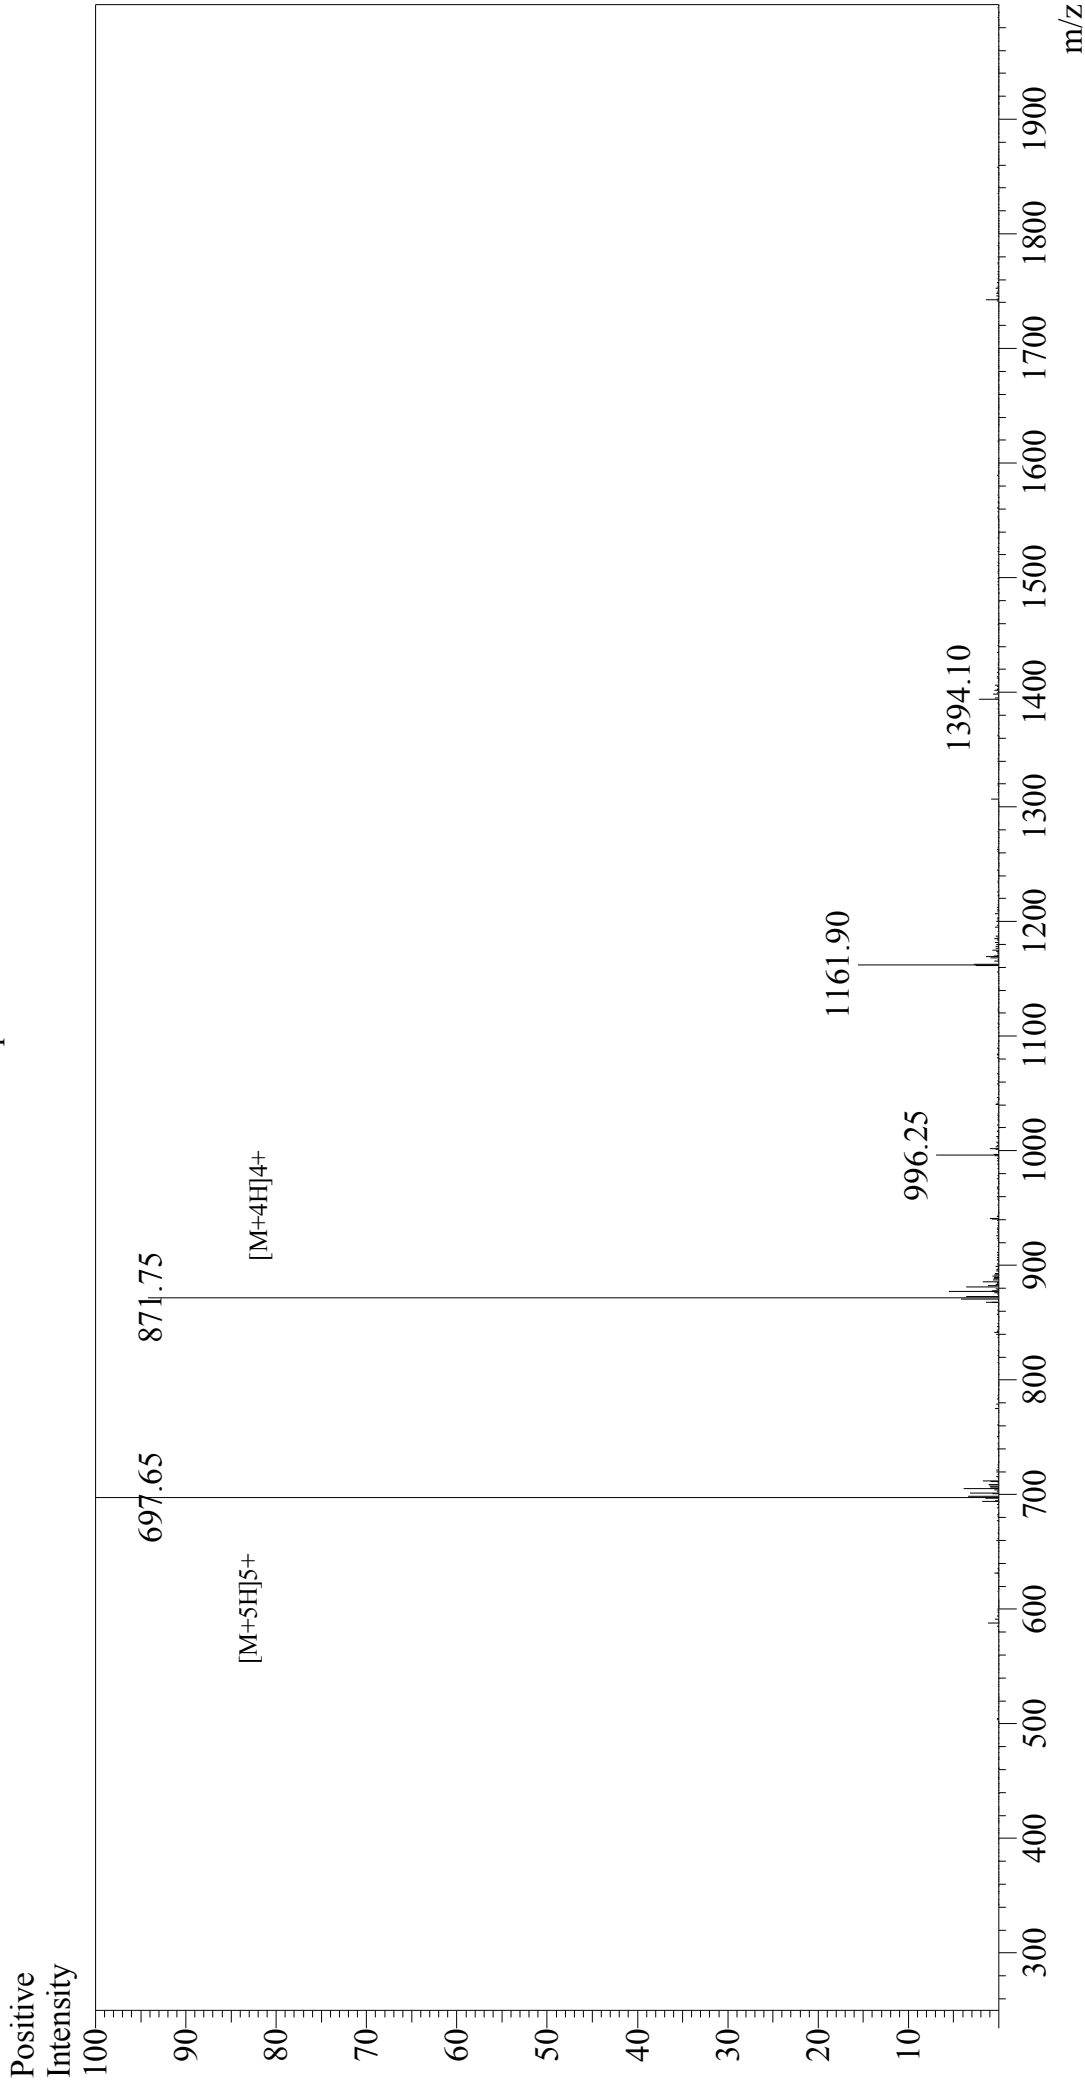

Sample Information

Acquired by : Gary
Month-Day Processed : 07/01/18
Time Processed : 17:42:01
Injection Volume : 0.2
Sample Name : Glucagon (1-29), Human, Hydrochloride Salt
Cat. No. : RP10772
Lot. No. : PE9821806
Theoretical MW : 3482.80
Observed MW : 3483.25

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H2O/50% MeOH