

Sample Name:CLIP (86-100)
 Cat No.: RP20279
 Lot No.:E2276820A
 Time Processed: 10:27:53
 Month-Day-Year Processed :01/14/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
35.00	Pumps	Solvent B Conc.	95
35.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : AlltimaTM C18 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

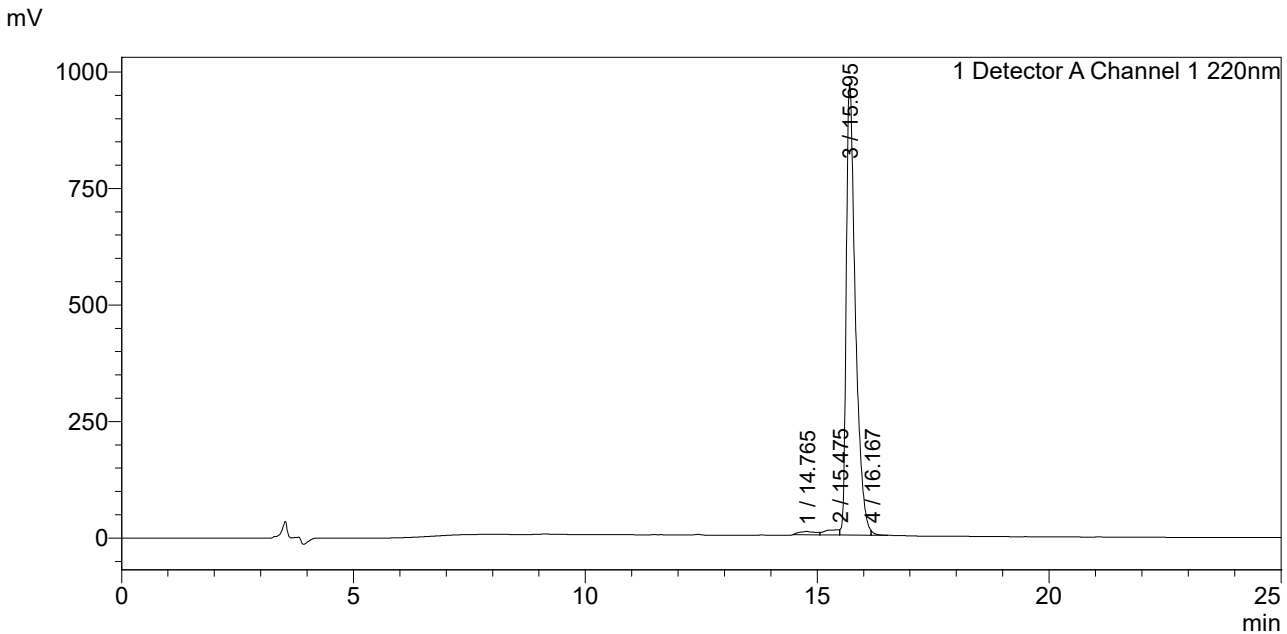

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.765	184772	7272	1.344
2	15.475	237928	11351	1.731
3	15.695	13279054	969815	96.617
4	16.167	42313	9109	0.308
Total		13744067	997547	100.000