

Sample Name :  $\beta$ -Amyloid (1-42), human  
 Cat. No. : RP10017  
 Lot. No. : E5731819K  
 Time Processed : 15:59:09  
 Month-Day-Year Processed : 12/25/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	10	
25.00	Pumps	Pump B Conc.	100	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	10	
40.00	Pumps	Pump B Conc.	10	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Boston Green C4 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

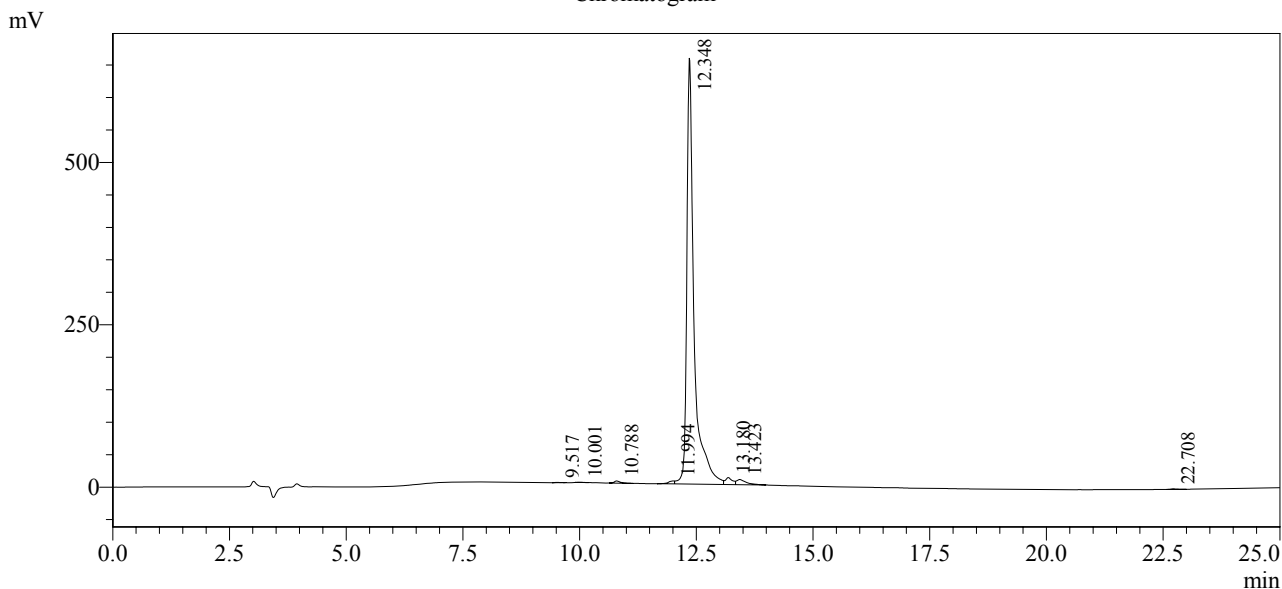

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.517	2754	381	0.038
2	10.001	3864	505	0.053
3	10.788	28651	3298	0.391
4	11.994	39842	4411	0.543
5	12.348	7024813	655718	95.817
6	13.180	114252	10663	1.558
7	13.423	111869	7958	1.526
8	22.708	5471	594	0.075
Total		7331516	683528	100.000