

Sample Name :CLIP (86-100)  
 Cat No. : RP20279  
 Lot No. : E8614920A  
 Time Processed :7:52:07  
 Month-Day-Year Processed :01/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

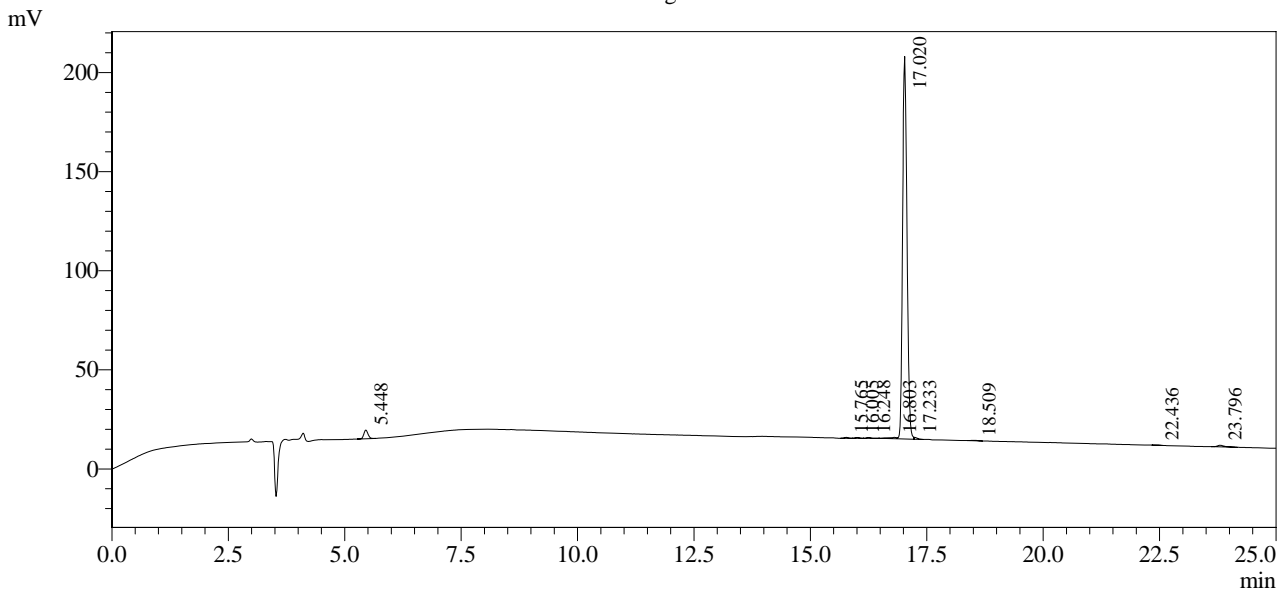

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.448	27317	4377	2.051
2	15.765	2807	463	0.211
3	16.005	2833	445	0.213
4	16.248	2727	447	0.205
5	16.803	8840	679	0.664
6	17.020	1270150	192987	95.360
7	17.233	4474	988	0.336
8	18.509	2001	214	0.150
9	22.436	1944	246	0.146
10	23.796	8854	824	0.665
Total		1331947	201669	100.000