

Sample Name :CLIP (86-100)
 Cat No.: RP20279
 Lot No.: PE8721902
 Time Processed : 17:32:57
 Month-Day-Year Processed :03/06/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

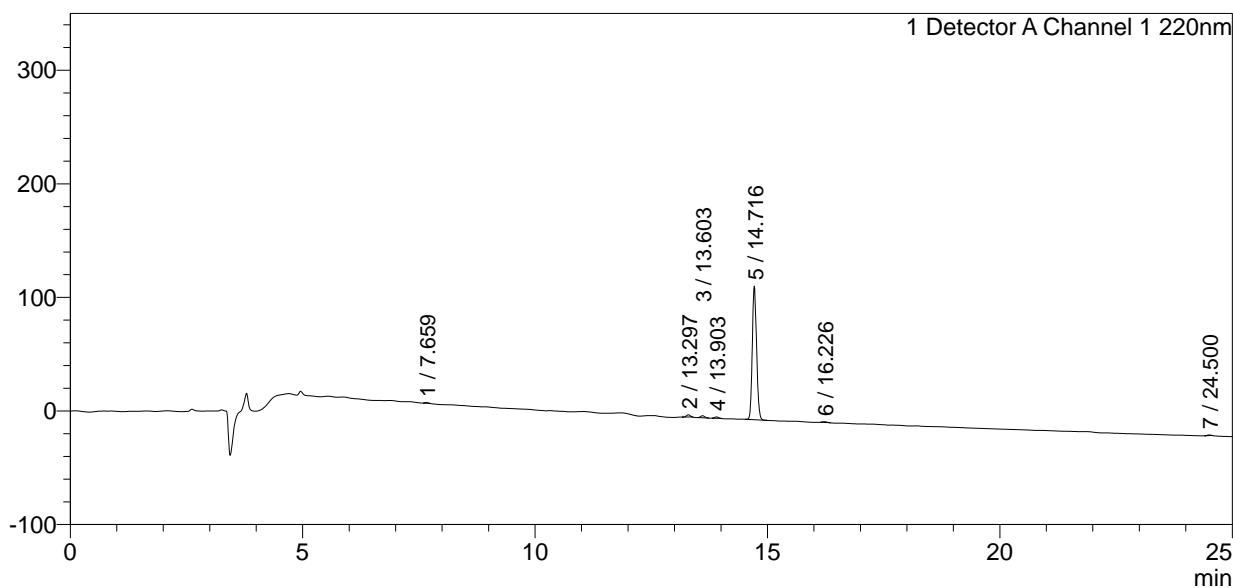

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.659	2555	689	0.322
2	13.297	10163	1881	1.280
3	13.603	10624	1791	1.338
4	13.903	6663	1220	0.839
5	14.716	757126	117703	95.328
6	16.226	4020	695	0.506
7	24.500	3082	582	0.388
Total		794234	124559	100.000