


Mass Spectrum

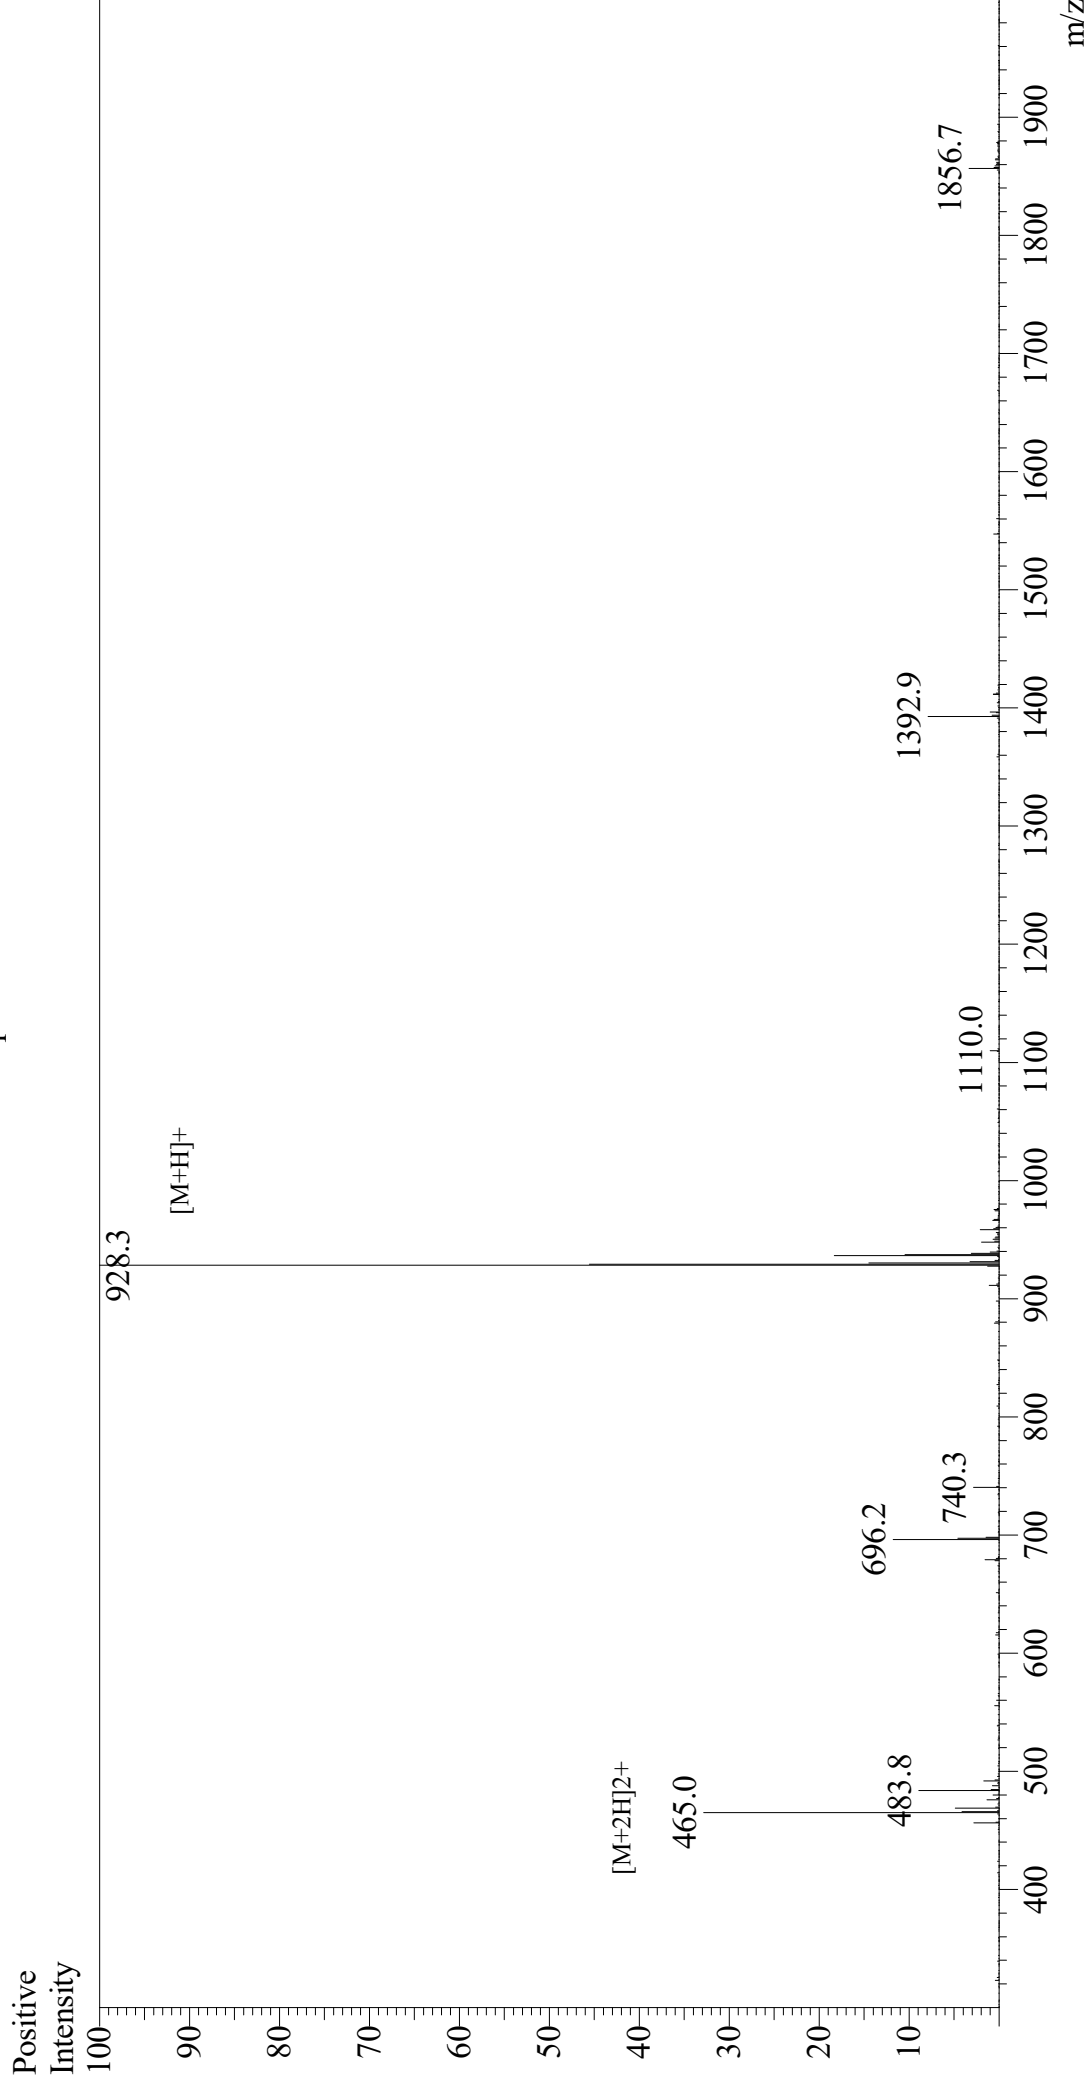

Sample Information

Acquired by : Gary
 Month-Day Processed : 02/23/20
 Time Processed : 05:33:25 PM
 Injection Volume : 0.5

Sample Name : Bacterial Sortase Substrate III, Abz/DNP
 Cat. No. : RP20431
 Lot. No. : E6692220B
 Theoretical MW : 928.00
 Observed MW : 927.3

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : GK11010007
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H₂O/50% MeOH