

Sample Name : Galanin, human  
 Cat No: RP10801  
 Lot No : E9397021G  
 Time Processed : 16:40:03  
 Month-Day-Year Processed : 07/16/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010140

<Chromatogram>

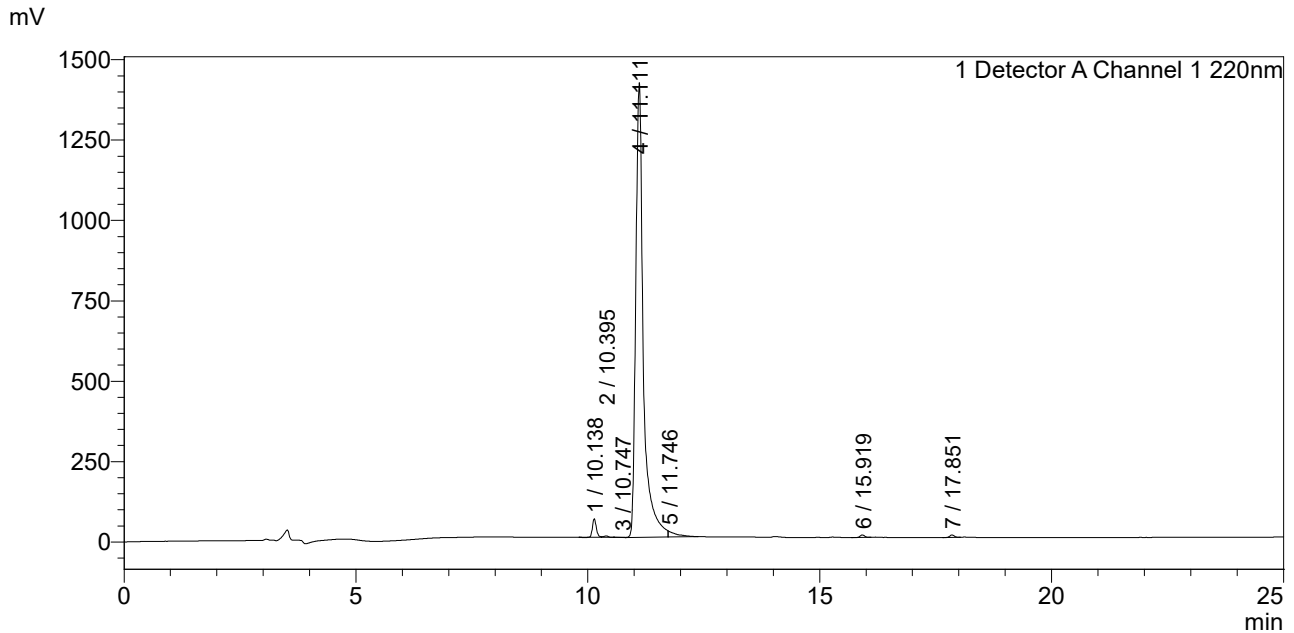

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.138	342120	57725	2.036
2	10.395	34422	4502	0.205
3	10.747	3065	596	0.018
4	11.111	16103342	1414477	95.854
5	11.746	215027	17995	1.280
6	15.919	49526	7705	0.295
7	17.851	52307	7806	0.311
Total		16799809	1510807	100.000