

Sample Name:  $\beta$ -Amyloid (4-10)  
 Cat No. : RP20173  
 Lot No. : E7039619J  
 Time Processed: 2:23:11 AM  
 Month-Day-Year Processed :10/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm  
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment:ZJ19010325

### <Chromatogram>

mV

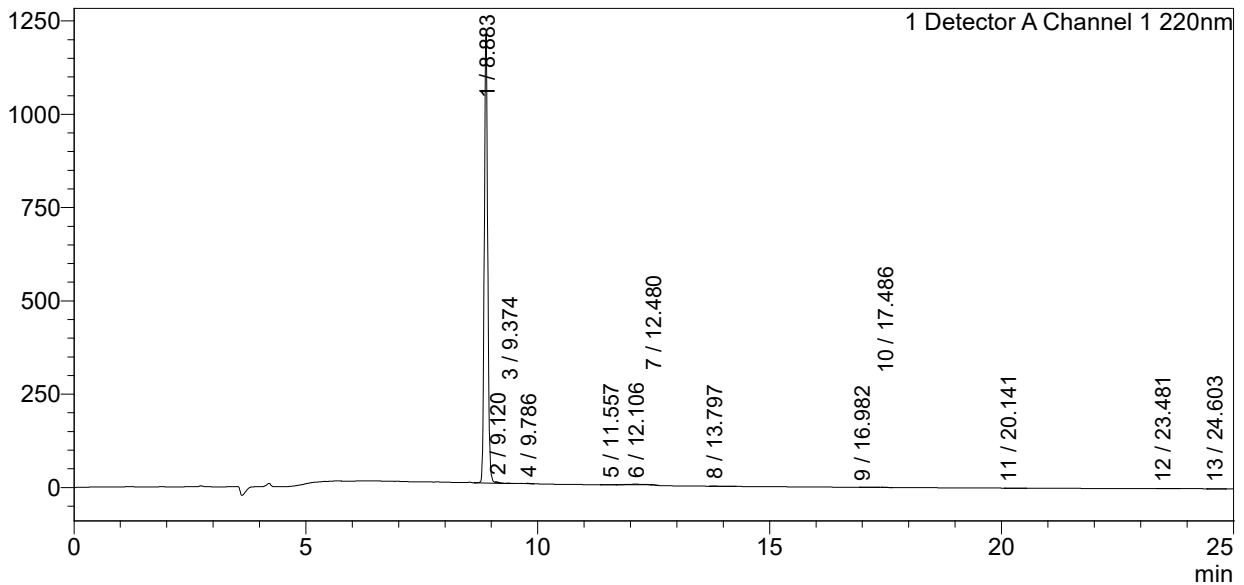

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.883	6138119	1202628	99.005
2	9.120	4295	1290	0.069
3	9.374	2402	507	0.039
4	9.786	6916	1257	0.112
5	11.557	2233	196	0.036
6	12.106	31036	1323	0.501
7	12.480	2540	609	0.041
8	13.797	6065	771	0.098
9	16.982	1069	43	0.017
10	17.486	1019	178	0.016
11	20.141	1522	75	0.025
12	23.481	1504	102	0.024
13	24.603	1093	85	0.018
Total		6199813	1209063	100.000