

Sample Name:[Des-Arg9]-Bradykinin
 Cat No. : RP13625
 Lot No. : E1544421G
 Time Processed : 4:11:51
 Month-Day-Year Processed : 07/13/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

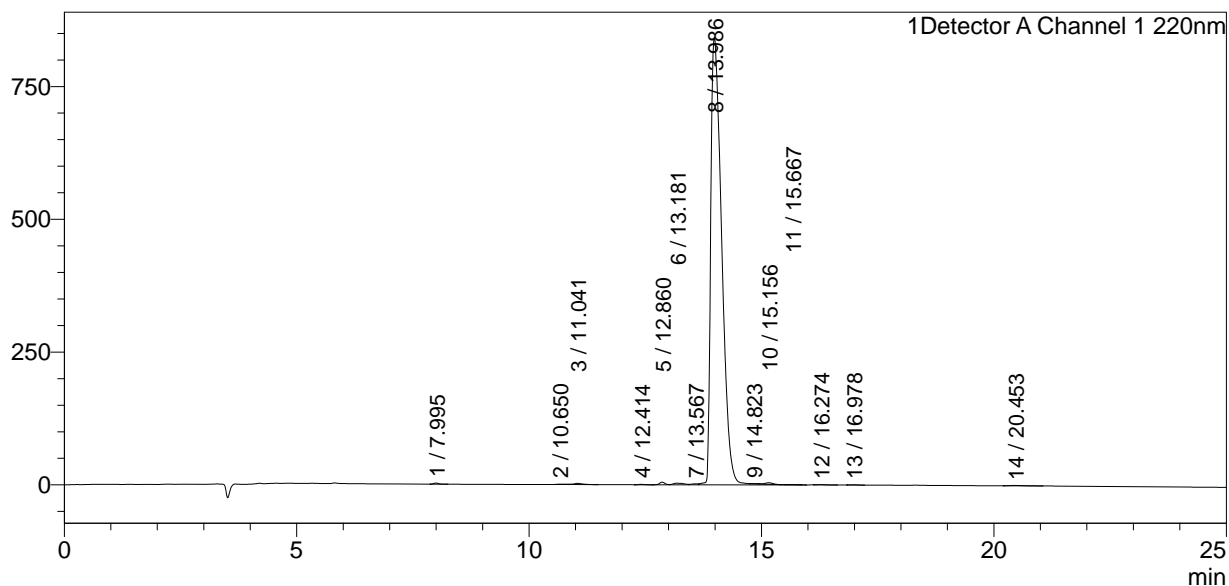

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.995	15543	2186	0.111
2	10.650	14674	679	0.105
3	11.041	29024	2258	0.207
4	12.414	7206	943	0.051
5	12.860	40076	4964	0.286
6	13.181	48329	3032	0.345
7	13.567	20677	1910	0.147
8	13.986	13777953	839639	98.247
9	14.823	5009	526	0.036
10	15.156	35027	2928	0.250
11	15.667	3718	423	0.027
12	16.274	5663	552	0.040
13	16.978	3627	426	0.026
14	20.453	17242	802	0.123
Total		14023770	861268	100.000