

Sample Name : Secretin, human  
 Cat No. : RP10249  
 Lot No. : E9400221D  
 Time Processed : 21:45:27  
 Month-Day-Year Processed : 04/21/2021  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment : SS-CM-0310

<Chromatogram>

mV

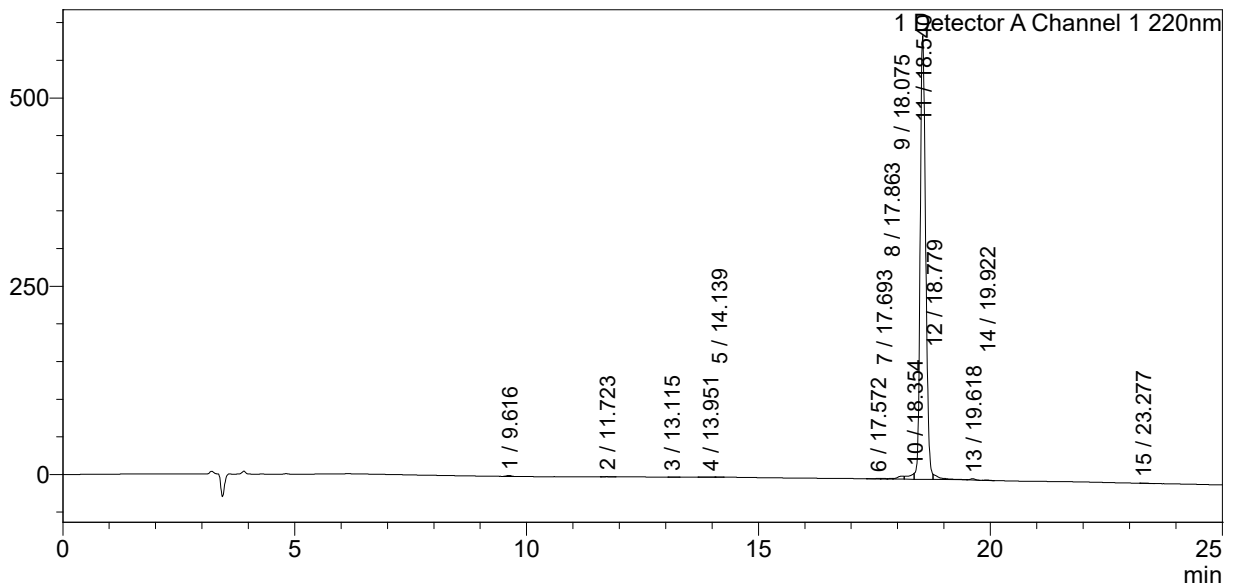

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.616	9538	1343	0.188
2	11.723	2854	318	0.056
3	13.115	1467	175	0.029
4	13.951	2622	205	0.052
5	14.139	1647	177	0.032
6	17.572	6060	655	0.119
7	17.693	4732	636	0.093
8	17.863	4999	713	0.099
9	18.075	38075	3823	0.750
10	18.354	64679	7451	1.275
11	18.540	4853607	589466	95.656
12	18.779	66421	6590	1.309
13	19.618	12523	1837	0.247
14	19.922	3614	553	0.071
15	23.277	1193	113	0.024
Total		5074031	614056	100.000