

Sample Name :SV40 T-Ag-derived NLS peptide  
 Cat No. :RP20513  
 Lot No. :E9092019I  
 Time Processed :12:49:48 PM  
 Month-Day-Year Processed :09/29/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

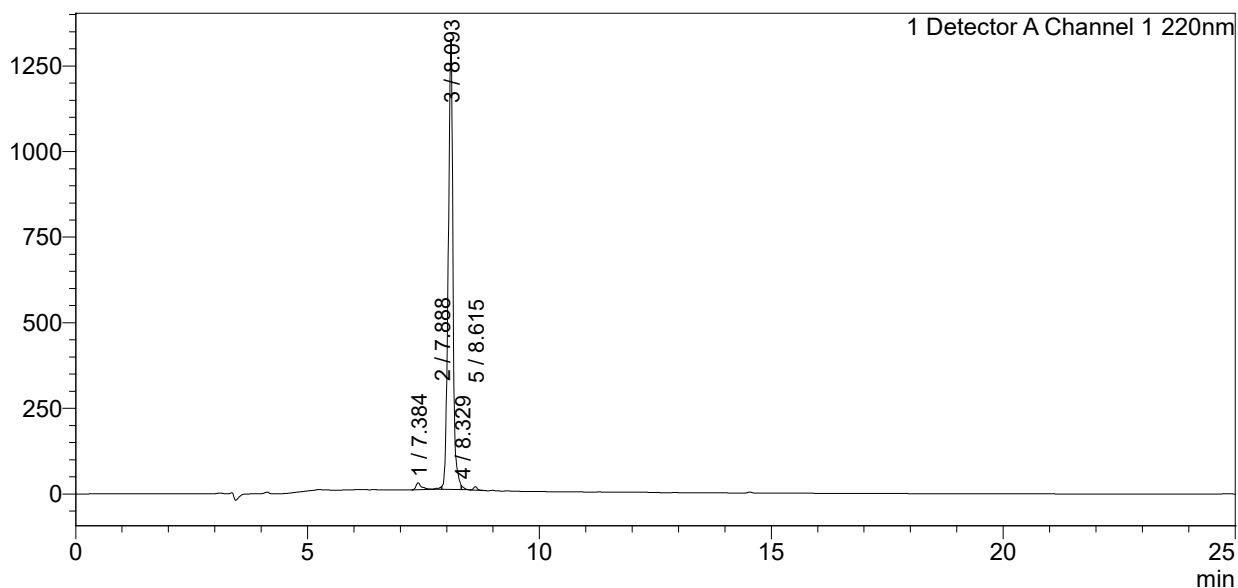

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.384	169452	20391	1.758
2	7.888	37979	7620	0.394
3	8.093	9343009	1315633	96.906
4	8.329	33050	10337	0.343
5	8.615	57812	10545	0.600
Total		9641302	1364526	100.000