

Sample Name :Amylin, human, amide
 Cat. No. : RP11278
 Lot. No. : PE7601809
 Time Processed :12:41:13
 Month-Day-Year Processed :10/26/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm
 Equipment:ZJ17010508

<Chromatogram>

mV

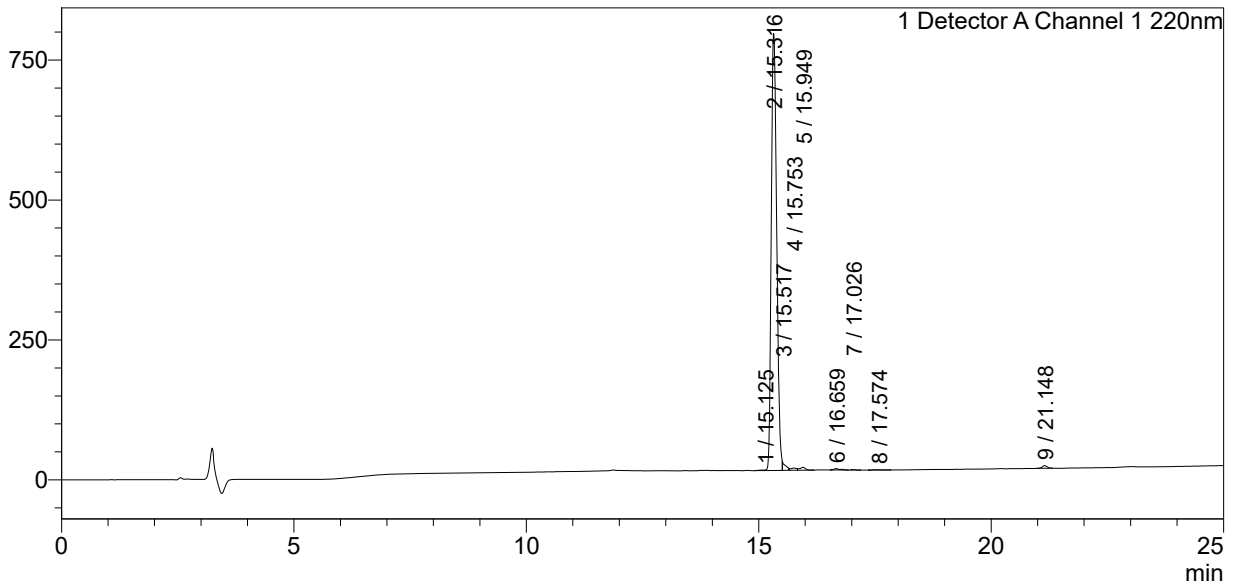

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.125	7047	824	0.108
2	15.316	6305770	780620	96.677
3	15.517	66255	13495	1.016
4	15.753	35484	3872	0.544
5	15.949	42359	5099	0.649
6	16.659	23037	2579	0.353
7	17.026	2057	528	0.032
8	17.574	7065	664	0.108
9	21.148	33448	4777	0.513
Total		6522522	812458	100.000