

Sample Name:LL37 (Human)
 Cat No :RP13323
 Lot No :E4434921E
 Time Processed :15:53:00
 Month-Day-Year Processed :05/29/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
30.00	Pumps	Pump A B.Conc	95
30.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

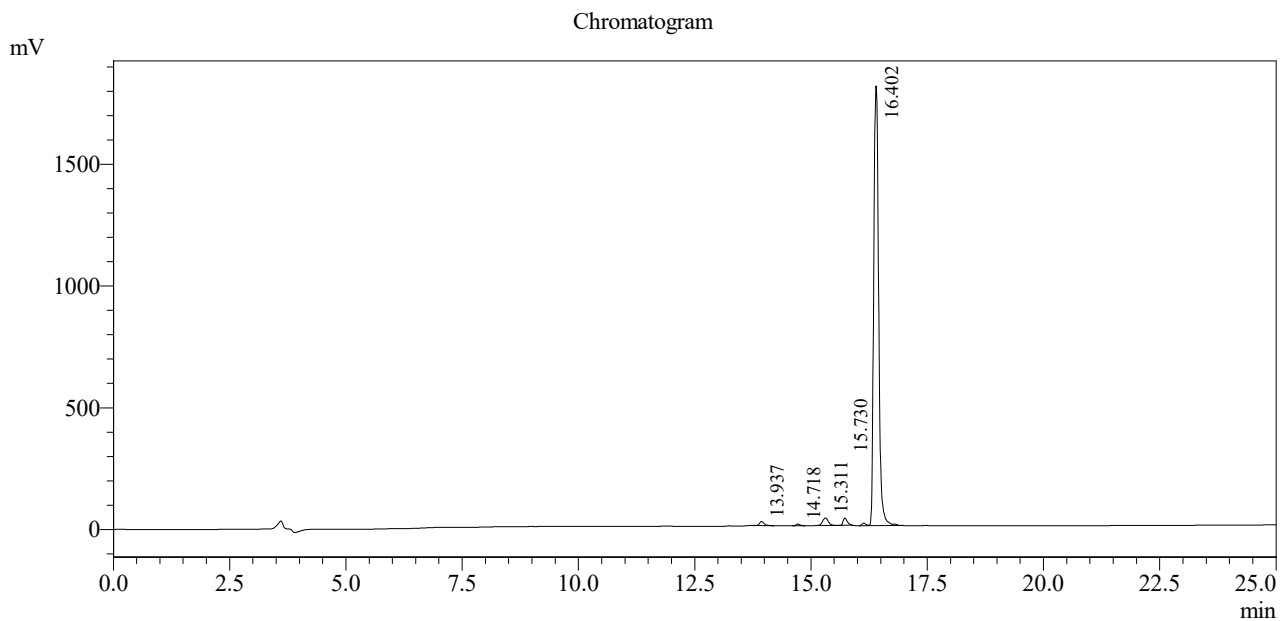

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.937	118437	16871	0.852
2	14.718	40248	7235	0.290
3	15.311	255110	30399	1.836
4	15.730	175967	29680	1.266
5	16.402	13305424	1806536	95.756
Total		13895186	1890721	100.000